

David Douce¹, Peter Hancock¹, Stephanie Dudd¹, Hans G.J. Mol²
¹Waters Corporation, Manchester M22 5PP, UK
²TNO, Zeist, The Netherlands

Introduction

There are over 800 registered pesticides in use worldwide, and an ever-increasing requirement to monitor the levels of these compounds in foodstuffs. Under EU legislation, maximum residue limits (MRLs) are specified for pesticides considered a potential health risk; guidelines for developing analytical methods must be followed.

The analytical challenge is to maximize the number of pesticides, minimize the variety of methods, keep run times short and achieve limits of detection (LoDs) at or below the reporting level. Multi-residue methods are efficient for analysis of pesticide residues. For methods with a very wide scope, generic sample preparation procedures are employed. Inherent to this approach is that clean up of extracts is only possible to a limited extent. When applying such methods to complex matrices like baby food, herbs, spices and tobacco, enhanced selectivity in detection is required to make up for the low selectivity in sample preparation.

Whereas single quadrupole and ion trap MS instruments are suitable for simple matrices where LoDs of >0.01 mg/kg are required, these detection

systems provide insufficient selectivity for complex food matrices, such as baby food, garlic, ginger, herbs and spices. In this work, gas chromatography (GC) with tandem quadrupole mass spectrometric detection (GC/MS/MS) was used to achieve the required selectivity.

Requirements of the analytical method:

- A simple and generic, rapid extraction method, allowing recovery of multiple classes of pesticides (OP, OC, pyrethroids, etc.)
- Analysis of 100 or more pesticides in 1 run
- LoDs at or lower than the reporting level
- Need for targeting multiple compounds in a variety of produce/matrices
- Efficient use of time/instrumentation/personnel (Multiresidue methods)
- Selective MS detection method (required to compensate for less selective sample prep)
- Adequate sensitivity to keep amount of (dirty!) matrix introduced into the GC system as low as possible



Figure 1. Waters® Micromass® Quattro micro™ GC.

Instrumentation

GC/MS/MS:	Waters® Micromass® Quattro micro™ GC
GC:	Agilent 6890 with PTV injector
Injection:	2 µl, solvent vent injection
Column:	30 m x 0.25 mm ID, 0.25 µm DB5MS
Carrier gas:	Helium, 1.0 mL/min (constant flow)
Temperature program:	50 °C (2 min) ramp 1 @25 °C/min – 150 °C ramp 2 @5 °C /min – 280 °C (4 mins) Total run time 36 mins
MS/MS:	Waters Micromass Quattro micro GC operated in Multiple Reaction Monitoring (MRM) mode
Ionization:	El positive ion
Q2 pressure:	2.5×10^{-3} mbar (argon)
Collision energy:	see Table 1
Sample preparation	
Sample amount:	2.5–25 g
Extraction:	50 ml ethyl acetate
Clean up:	PSA and GCB (dispersive)
Final extract:	0.05–0.5 g/ml

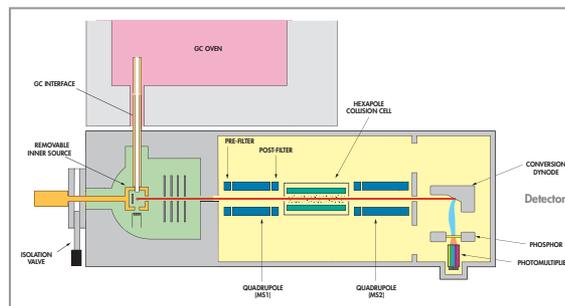


Figure 2. Waters Micromass Quattro micro GC instrument schematic.

Method development

In order to maximize the response of the instrument for each residue the choice of precursor ion, product ion and collision energy were optimized.

Initially, the pesticide mixture was analysed in full scan mode (Figure 3).

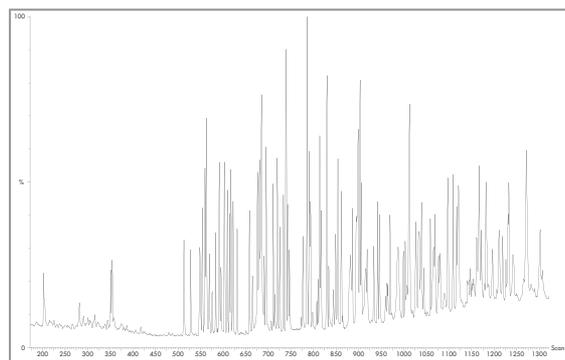


Figure 3. GC/MS full scan chromatogram (solvent standard of 100 pesticides).

Pesticide	Retention time	Precursor ion	Product ion	Collision energy (V)	Corr.coef. (r ²)	LOD (pg)	Pesticide	Retention time	Precursor ion	Product ion	Collision energy (V)	Corr.coef. (r ²)	LOD (pg)
dichlorvos	7,08	185	93	12	0,998	3	dieldrin	21,04	237	165	20	0,976	5
mevinphos-cis	8,68	192	127	10	0,994	1	TDE, o,p'	21,15	235	165	15	0,973	3
mevinphos-trans	8,72	192	127	10	0,995	1	cinerin-I	21,47	123	81	7	0,997	4
ethoprophos	11,60	158	114	5	0,999	4	endrin	21,78	263	193	25	0,994	17
chlorpropham	11,93	213	171	5	0,998	4	nitrofen	21,81	283	253	10	0,998	30
cadusafos	12,40	159	131	5	0,998	5	endosulfan-beta	22,20	237	143	25	0,983	22
phorate	12,51	260	75	5	0,906	26	fensulfathion	22,28	292	109	10	0,993	9
HCH-alfa	12,65	181	145	10	0,997	8	TDE, p,p'	22,45	235	165	15	0,999	1
hexachlorobenzene	12,73	284	249	15	0,999	2	DDT, o,p'	22,54	235	165	15	0,981	4
dimethoate	13,05	229	87	5	0,996	12	ethion	22,55	231	129	20	0,993	2
carbofuran	13,26	164	149	8	0,998	3	jasmolin-I	22,80	164	109	8	0,996	17
HCH-beta	13,48	181	145	10	0,999	4	triazophos	23,12	257	162	5	0,994	11
dimethipin	13,48	118	58	7	0,997	25	carbophenothion	23,47	342	157	10	0,991	8
quintozene	13,51	295	237	15	0,997	11	endosulfan-sulphate	23,60	387	241	15	0,986	44
lindane	13,70	181	145	10	0,997	5	DDT-p,p'	23,83	235	165	20	0,971	4
diazinone	14,12	179	137	15	0,995	15	propargite	24,51	135	107	12	0,998	9
chlorothalonil	14,22	266	133	25	0,996	5	piperonylbutoxide	24,79	176	131	10	0,993	4
pentachloroaniline	15,14	165	194	20	0,995	5	pyrethrin-I	25,20	133	105	8	0,999	12
phosphamidon	15,43	264	127	10	0,995	8	phosmet	25,49	160	77	20	0,990	3
chlorpyrifos-methyl	15,66	286	93	18	0,995	4	bromopropylate	25,71	341	183	15	0,996	2
vinclizolin	15,82	212	145	20	0,998	6	fenpropathrin	26,09	181	152	20	0,996	4
parathion-methyl	15,89	263	127	8	0,990	6	tetradifon	26,60	229	201	12	0,999	4
alachlor	15,93	188	160	8	0,994	3	phosalone	26,86	182	111	10	0,994	5
carbaryl	16,10	144	115	20	0,997	2	phenothrin	26,86	183	153	12	0,993	11
heptachlor	16,12	272	237	10	0,994	2	azinphos-methyl	26,95	160	132	5	0,987	11
pirimiphos-methyl	16,73	290	125	15	0,999	3	cinerin-II	27,05	169	107	5	0,997	90
MPCPS	16,84	296	263	12	0,998	2	cyhalothrin-lambda	27,73	197	141	10	0,996	3
malathion	17,16	173	99	10	0,997	3	azinphos-ethyl	28,17	160	132	5	0,992	3
chlorpyrifos	17,34	197	169	20	0,994	8	acrinathrin	28,17	181	152	18	0,994	6
aldrin	17,36	263	193	22	0,991	7	jasmolin-II	28,25	163	121	6	0,995	23
fenthion	17,50	278	109	12	0,929	10	permethrin-cis	29,23	183	153	12	0,996	4
parathion	17,64	291	109	10	0,986	21	permethrin-trans	29,50	183	153	12	0,997	3
fenpropimorf	17,66	303	128	5	0,985	6	prochloraz	29,51	180	152	20	0,989	47
triadimefon	17,75	208	181	6	0,996	6	cyfluthrin I	30,33	163	127	5	0,997	2
chlordane, oxy	18,76	185	121	10	0,998	5	cyfluthrin II	30,55	163	127	5	0,996	1
fipronil	18,76	367	213	25	0,996	5	cyfluthrin III	30,64	163	127	5	0,994	3
heptachlor-epoxide	18,90	353	257	15	0,994	11	cyfluthrin IV	30,75	163	127	5	0,993	5
chlorfenvinphos	18,94	325	269	10	0,991	8	cypermethrin I	30,97	163	127	5	0,993	2
phenthoate	19,10	274	121	7	0,995	5	cypermethrin II	31,18	163	127	5	0,996	3
quinalphos	19,13	146	118	7	0,996	2	cypermethrin III	31,28	163	127	5	0,995	2
triadimenol	19,27	168	70	5	0,990	31	flucythrinate I	31,32	199	157	5	0,994	1
methidathion	19,59	145	85	5	0,996	1	cypermethrin IV	31,38	163	127	5	0,997	2
chlordane-alfa	19,61	373	266	15	0,995	5	etofenprox	31,59	163	135	10	0,997	1
tetrachlorvinphos	19,87	329	109	18	0,994	3	flucythrinate II	31,73	199	157	5	0,997	1
endosulfan-alfa	20,06	237	143	25	0,998	16	fenvaleate I	32,71	167	125	8	0,997	2
chlordane-gamma	20,07	373	266	15	0,995	24	fluvalinate,tau-	33,03	250	200	20	0,998	17
prothiofos	20,66	267	239	5	0,989	6	fenvaleate II	33,18	167	125	8	0,997	4
profenofos	20,85	337	267	8	0,992	5	fluvalinate,tau-	33,22	250	200	20	0,994	4
DDE, p,p'	20,95	246	176	22	0,997	1	deltamethrin	34,48	181	152	18	0,998	6

Table 1. Precursor and products ions, linearity and LoDs.

The precursor ion was selected from the full scan spectra based on its relative abundance, e.g. Endosulfan-beta (MW = 404; Figure 4).

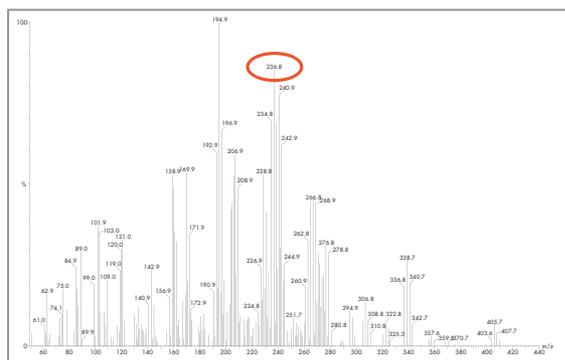


Figure 4. Full scan background subtracted spectrum of Endosulfan-beta.

The collision energy for the product ion was optimised using a range of collision energies between 5–30 eV (Figure 5).

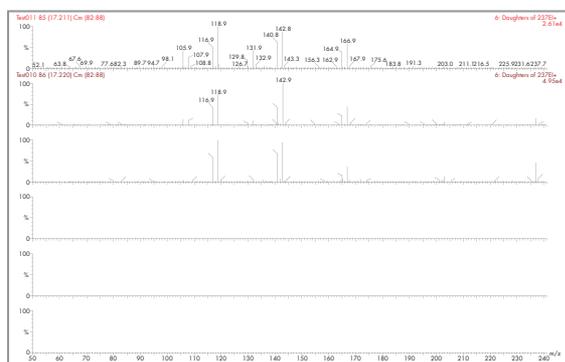


Figure 5. MS/MS optimization.

Method Performance

For the majority of pesticides, LoDs were below 10 pg on column (based on S/N >3:1; Table 1).

The ability to quantify closely eluting peaks is a prerequisite of multiresidue methods. Therefore, the dwell time allocated for each transition must be sufficient to ensure that at least 10 data points are acquired for accurate quantification. To assess the effect of short dwell times on data quality a standard solution of hexachlorobenzene was acquired using a range of dwell times.

Figure 6 illustrates that the signal intensity is unaffected by the shorter dwell time. With a 10 ms dwell time, the S/N measured is sufficient for quantification of the target compounds.

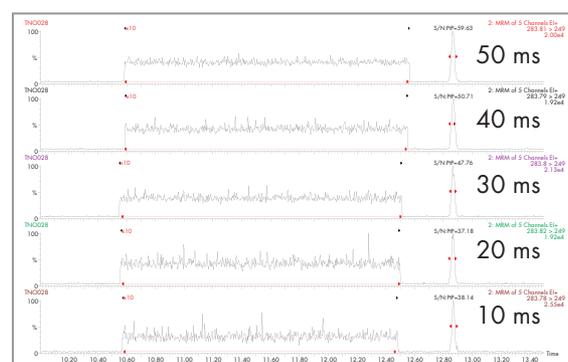


Figure 6. 2 µl standard solution of hexachlorobenzene (10 pg/µl) acquired using a range of dwell times, from 10–50 ms.

To assess instrument robustness, hexachlorobenzene (20 pg on-column) was analyzed repeatedly (n = 10) at a range of different dwell times, from 10–50 ms. The % RSD shown in Table 2 illustrates the repeatability of injection was less than 5%.

Hexachlorobenzene (20 pg)	
Dwell (ms)	% RSD (n = 10)
10	3.0
20	4.4
30	3.9
40	2.5
50	2.8

Table 2. Effect of dwell time on repeatability.

For 100 pesticide residues, the optimum experimental setup utilized 84 MRM transitions in 14 MRM function windows, with 4 to 8 transitions in each window (Figure 7). With this setup, at any point in time, the maximum number of transitions acquired was 15.

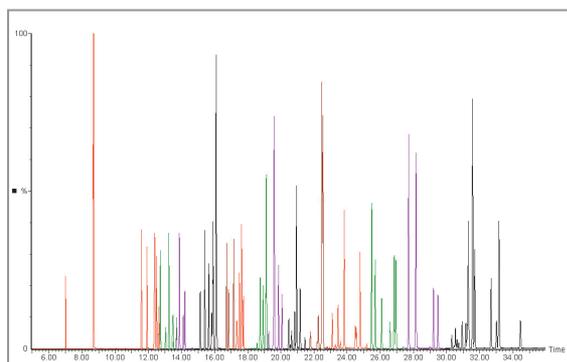


Figure 7. TIC of 100 pesticides in MRM mode. Each color corresponds to a different function window.

The linearity of the system is illustrated in Figure 8.

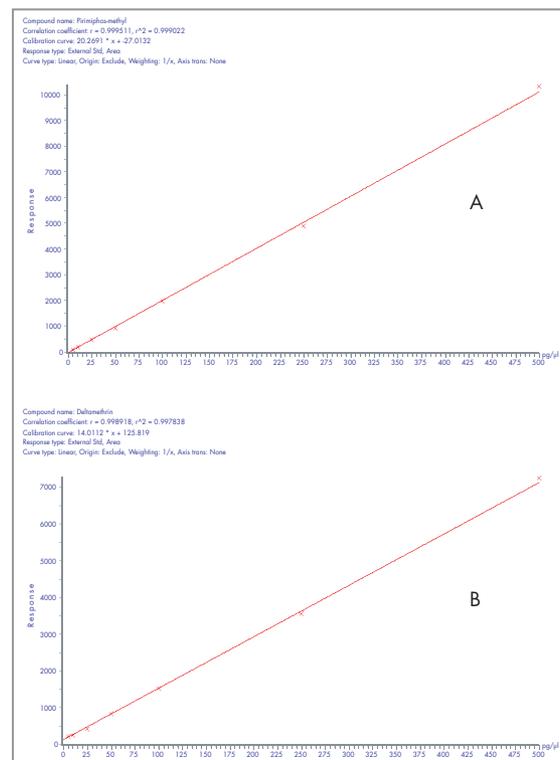


Figure 8. Calibration curves for A) Pyrimiphos-methyl ($T_r = 16.73$ mins) and B) Deltamethrin ($T_r = 34.48$ mins) showing linearity over the concentration range.

Results

The analytical method was applied to the analysis of a range of complex food extracts, including fresh produce, baby food (matrix equivalent = 0.5 g/ml), dried herbs, spices, tobacco, ginkgo and cannabis (matrix equivalent = 0.1 g/ml).

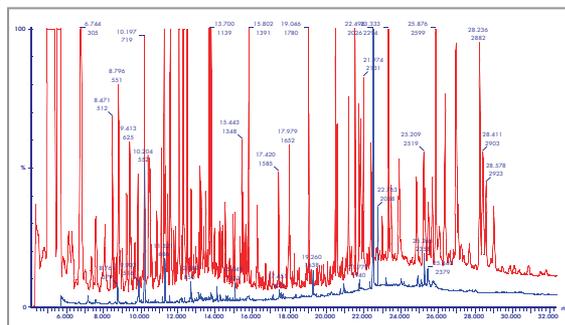


Figure 9. GC full scan chromatograms (TIC) of herbal tea, 0.2 mg on column (red trace) and strawberry, 10 mg on column (blue trace).

Figure 9 compares chromatograms from complex and non-complex matrices, showing the importance of high selectivity for the analysis of these types of sample. Figure 10 shows the GC/MS/MS chromatograms of selected pesticide residues in herbal tea.

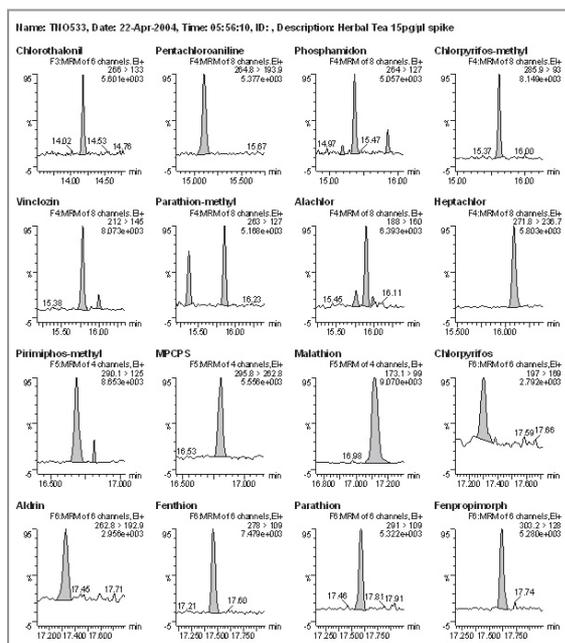


Figure 10. GC/MS/MS of selected pesticides in herbal tea (0.3 mg/kg dry).

In all cases (Table 3), a high percentage of the spiked pesticides were detected and measured, despite the highly complex matrices, generic sample preparation and limited clean up employed.

Product	Pesticide fortification	Compounds spiked	Compounds found	% found
Baby food	0.01 mg/kg	93	81	87
Baby food	0.05 mg/kg	93	92	99
Herbal tea	0.03 mg/kg	93	88	95
Herbal mix	0.03 mg/kg	93	87	94
Curry	0.15 mg/kg	93	90	97
Massala	0.15 mg/kg	93	87	94
Tobacco	0.15 mg/kg	93	87	94
Ginko	0.02–4.0 mg/kg	52	44	85
Cannabis	0.02–4.0 mg/kg	52	41	79

Table 3. Summary of performance in terms of selectivity.

Conclusions

- A multiresidue method has been developed for the surveillance monitoring of 100 pesticide residues in a range of food matrices.
- Sufficient selectivity has been achieved to allow generic sample clean up, even for very complex food matrices.
- The Waters Micromass Quattro micro GC can be used in routine analysis at 10 ms dwell times. Subsequent expansion of this method to include an increased number of MRM transitions would be possible without a loss in sensitivity.
- The system provided good sensitivity (1–10 pg on column) for the majority of pesticide residues, allowing the amount of matrix introduced into the GC system to be minimized.

Sales Offices:

AUSTRIA 43 1 877 18 07

AUSTRALIA 61 2 9933 1777

BELGIUM AND LUXEMBOURG 32 2 726 1000

BRAZIL 55 11 5543 7788

CANADA 800 252 4752 X2205

CZECH REPUBLIC 420 2 617 11384

DENMARK 45 46 59 8080

FINLAND 358 9 506 4140

FRANCE 33 1 3048 7200

GERMANY 49 6196 400600

HONG KONG 852 29 64 1800

HUNGARY 36 1 350 5086

INDIA 91 80 2837 1900

IRELAND 353 1 448 1500

ITALY 39 02 27 4211

JAPAN 81 3 3471 7191

KOREA 82 2 820 2700

MEXICO 52 55 5524 7636

THE NETHERLANDS 31 76 508 7200

NORWAY 47 6 384 6050

PEOPLE'S REPUBLIC OF CHINA 86 10 8451 8918

POLAND 48 22 833 4400

PUERTO RICO 787 747 8445

RUSSIA/CIS 7 095 931 9193

SINGAPORE 65 6278 7997

SPAIN 34 93 600 9300

SWEDEN 46 8 555 11 500

SWITZERLAND 41 62 889 2030

TAIWAN 886 2 2543 1898

UK 44 208 238 6100

US 800 252 4752

Waters

WATERS CORPORATION

34 Maple St.

Milford, MA 01757 U.S.A.

T: 508 478 2000

F: 508 872 1990

www.waters.com

For Complete Confidence

Waters, Micromass and Quattro micro are trademarks of Waters Corporation.
All other trademarks are property of their respective owners.
©2004 Waters Corporation Printed in the U.S.A. October 2004 720000987EN LL-PDF



001