

A Modular Preparative HPLC System for the Isolation of Puerarin from Kudzu Root Extracts

Andrew Aubin and Ronan Cleary
Waters Corporation, Milford, MA, USA

APPLICATION BENEFITS

A modular preparative HPLC system provides flexibility without compromising performance for isoflavone isolation. Empower™ 2 Software offers total system control including fraction collection.

WATERS SOLUTIONS

Component-based preparative HPLC modules

Empower 2 Software

SunFire™ Columns

KEY WORDS

Preparative HPLC, Kudzu, Puerarin

INTRODUCTION

Kudzu (*Pueraria lobata*) is a climbing, woody, or semi-woody perennial vine with a tuberous root. The roots of kudzu contain a number of potentially useful isoflavones, including daidzein, daidzin, genistein, genistin, and quercetin. Kudzu is also a unique source of the isoflavone puerarin as shown in Figure 1. Consumption of kudzu root extracts is thought to reduce alcohol intake and reduce alcohol withdrawal symptoms. Antibacterial, anti-cancer, anti-inflammatory, and antioxidant effects have also been noted.¹

Generally, the goal in natural product purification is to isolate individual component compounds that may have biological activity. Sufficient amounts of these potentially active compounds need to be isolated in order to facilitate characterization of unknown compounds or for use in other studies, such as clinical trials and bioassays. The isolated compounds must be of high purity so that any results obtained can be attributed to the compound under study rather than small amounts of companion compounds. Many techniques for extraction, isolation, and purification of natural products have been previously described.²

Preparative reversed-phase high performance liquid chromatography (RP-HPLC) is a separation technique that is widely used in this endeavor. It is considered a rapid, reliable, and robust technique that has wide applicability over many classes of compounds. This application note describes the isolation of the isoflavone puerarin from the roots of the kudzu plant using a modular preparative HPLC system.

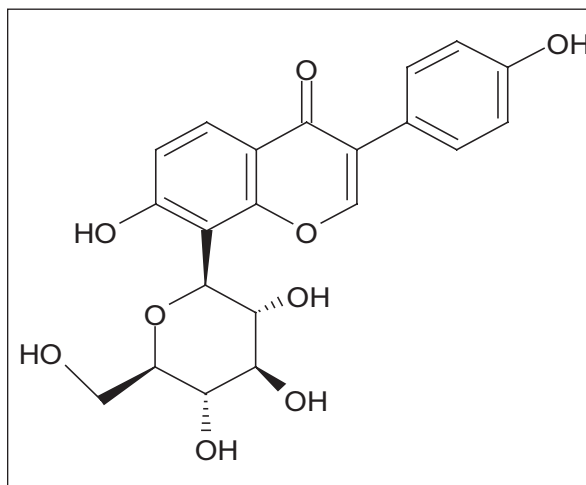


Figure 1. Chemical structure of puerarin.

EXPERIMENTAL

Extraction

Kudzu root powder (50 g) was added to 250 mL of 9:1 water/methanol and shaken for one hour, allowed to stand overnight, and shaken for an additional hour. This extract was centrifuged at 3000 RPM for 20 minutes, passed through Whatman #1 filter paper, and used without further treatment.

Separation

Preparative chromatographic separations were carried out using a Waters® Modular HPLC System as shown in Figure 2, which consisted of the following components:

Pump: 2535 Quaternary Gradient Module
 Detector: 2489 UV/Visible Detector
 Injector: 2707 Autosampler configured with a 1-mL loop
 Collector: Fraction Collector III
 Columns: Initial Prep Trial – SunFire C₁₈, 5 µm, 10 x 100 mm
 Final Prep Method – SunFire C₁₈, 5 µm, 19 x 100 mm Column



Figure 2.
Waters Modular
Preparative
HPLC System.

Analytical chromatographic separations, implemented for method development and final purity checks, were carried out using the Alliance® HPLC 2695 and a 2998 PDA Detector with a SunFire C₁₈, 5 µm, 4.6 x 100 mm Column. Both the analytical and prep systems, including fraction collection, were controlled using Empower 2 Software to collect, manage, process, and report chromatography data. Two initial analytical scale separations were developed (one gradient for purity checks and one isocratic for purification) with the conditions described on the next page.

RESULTS AND DISCUSSION

Gradient HPLC analysis of the prepared extract indicated a puerarin concentration of ~0.5 mg/mL and an overall purity of 59.6% by UV area percent as shown in Figure 3. Using a previously developed analytical isocratic HPLC method (data not shown), the separation was scaled to the 10-mm I.D. prep column using the Preparative OBD™ Column Calculator shown in Figure 4. The Preparative OBD Column Calculator, a free download, provides an easy-to-use tool that aids in analytical-to-preparative scaling calculations (www.waters.com/prepcalculator). The Preparative OBD Column Calculator was used to convert the analytical separation method to the preparatory separation methods described in this application note. The use of the Preparative OBD Column Calculator has been described in a previous application note.³

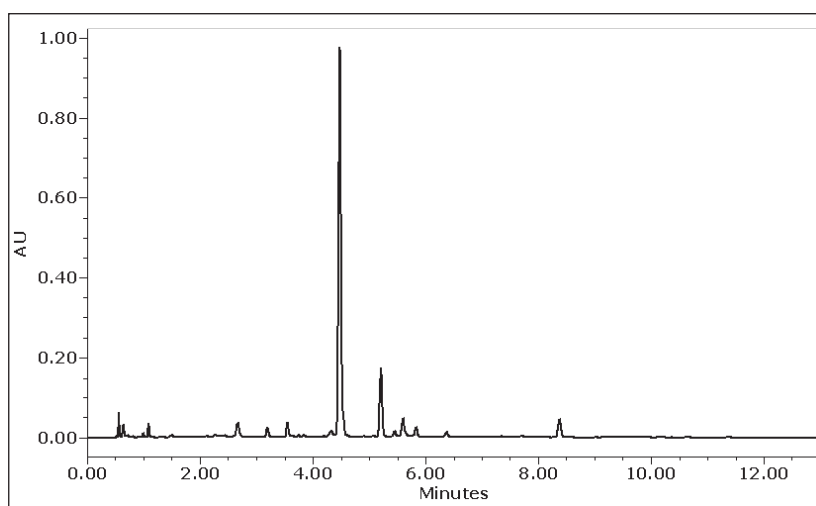


Figure 3. Analytical gradient separation of kudzu root extract.

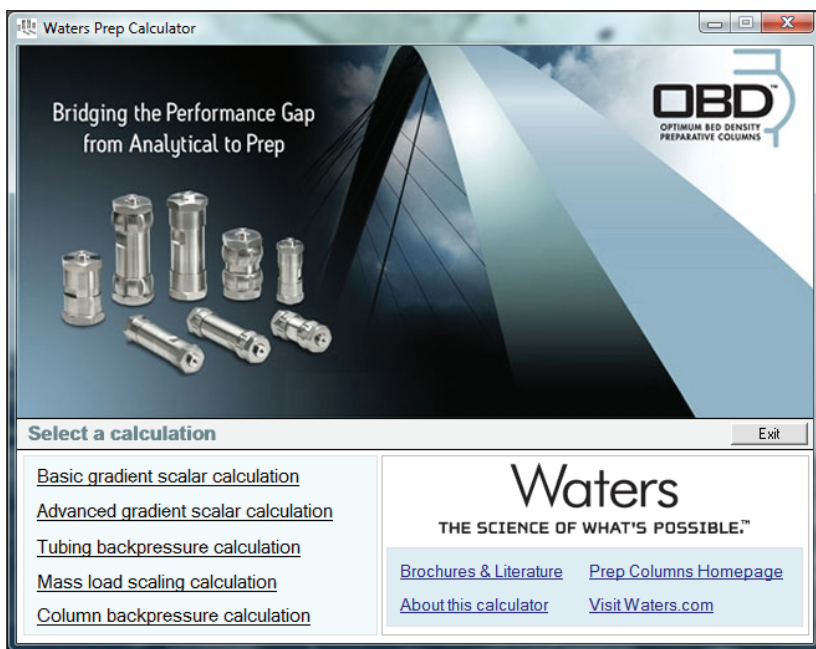


Figure 4. Waters Preparative OBD Column Calculator.

Analytical Gradient Conditions

Column temp.:	Ambient
Flow rate:	1.5 mL/min
Mobile phase A:	Water + 0.1% formic acid
Mobile phase B:	Acetonitrile
Gradient:	95% A:5% B to 20:80 over 20 minutes
Detection:	UV at 251 nm

Analytical Isocratic Conditions

Column temp.:	Ambient
Flow rate:	1.5 mL/min
Mobile phase A:	88.5% Water + 0.1% formic acid
Mobile phase B:	11.5% Acetonitrile
Detection:	UV at 251 nm

Preparative separations were geometrically scaled from the analytical methods and are described below.

Preparative Isocratic Conditions

Column temp.:	Ambient
Flow rate:	7 or 25 mL/min (for 10 and 19 mm I.D. respectively)
Mobile phase A:	88.5% Water + 0.1% formic acid
Mobile phase B:	11.5% Acetonitrile
Injection vol.:	500 μ L using Autosampler with 10-mm column or 2000 μ L using Line D of the 2535 with 19-mm column
Detection:	UV at 251 nm

Using a 500- μ L injection, acceptable reproducible preparative separations were achieved at 2.1% RSD retention time, as indicated in Figure 5. In order to increase the throughput, the method was further scaled to a 19-mm I.D. column. Injection volume scaling calculations indicated that a 2-mL injection was needed to keep the chromatography constant. Because the 2707 Autosampler was configured with a 1-mL loop, sample loading via the D line of the 2535 Quaternary Pump was used. In this loading technique, sample was introduced using a gradient table outlined in Figure 6. The gradient method was initiated via Empower 2 Software using the "Inject Immediate Sample Function." Although the Autosampler is not used, it does not have to be removed from the system, which allows users to quickly choose sample introduction via the pump or autosampler.

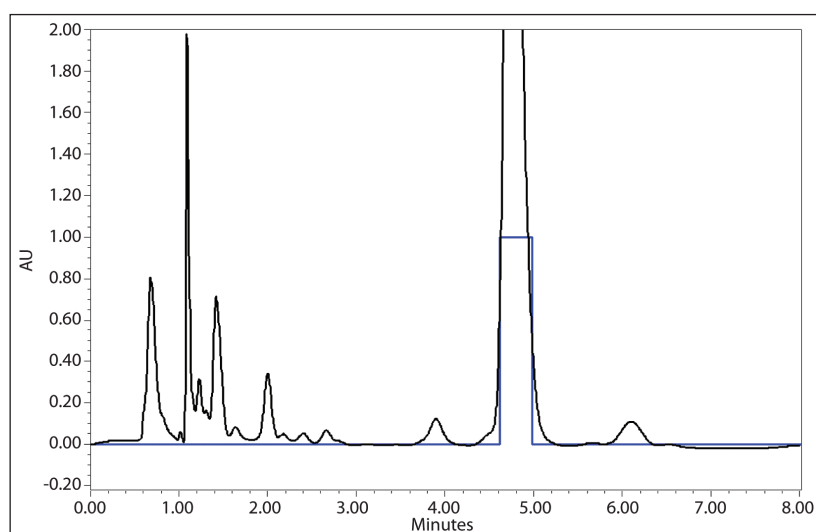


Figure 5. Prep (10 mm I.D.) separation of kudzu root extract using autosampler injection (black line is the UV output, blue line is the fraction collector state, 0.0=off, 1.0=on).

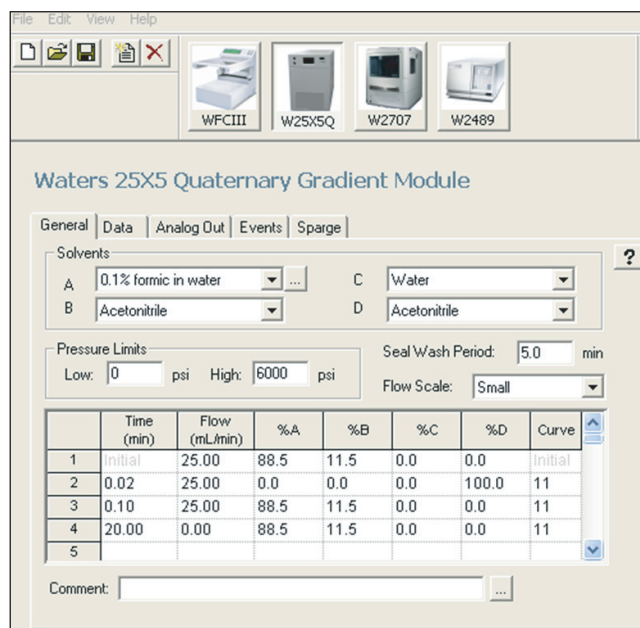


Figure 6. Empower Gradient Table with "Line D" loading.

Acceptable, reproducible prep separations were again achieved with the 19-mm column shown in Figure 7. Fraction collection was set up using Empower 2 Software for threshold collection within a window. In this mode, a collection window is defined (in this case 3.0 to 6.0 minutes), and any peaks eluted outside of that window are not collected. Peaks eluting within the window must meet peak threshold criteria (in this case ~ 0.60 AU) to be collected. In addition, the fraction collector was set to collect multiple injections per position. Each peak is collected into the same bed position, as opposed to each peak being collected into a separate container. This allows for bulk-style purification and eliminates the need to pool collected fractions from identical sample injections. Ten separate injections totaling ~ 11.5 mg of puerarin were made on the 19-mm column with a total volume collected of 92 mL. Subsequent analysis of the collected fractions shown in Figure 8 had a puerarin concentration of 0.099 mg/mL with a UV area purity of $>97.5\%$. The overall yield of puerarin from the kudzu extract was 79.6%.

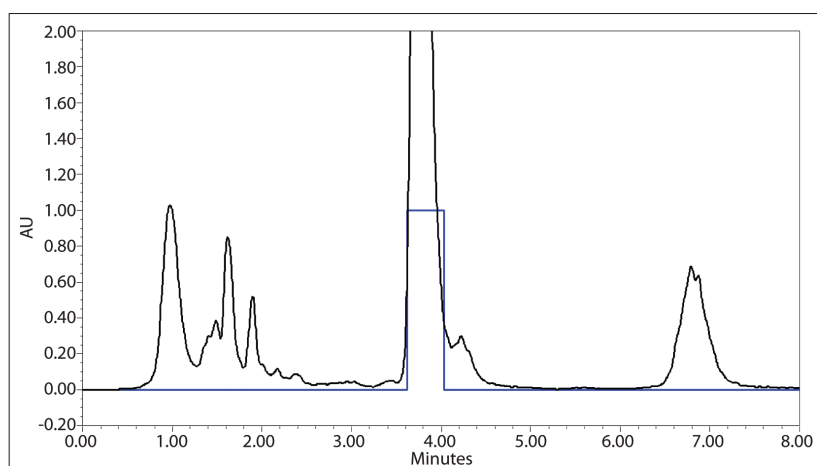


Figure 7. Prep (19 mm I.D.) separation of kudzu root extract using "Line D" loading.

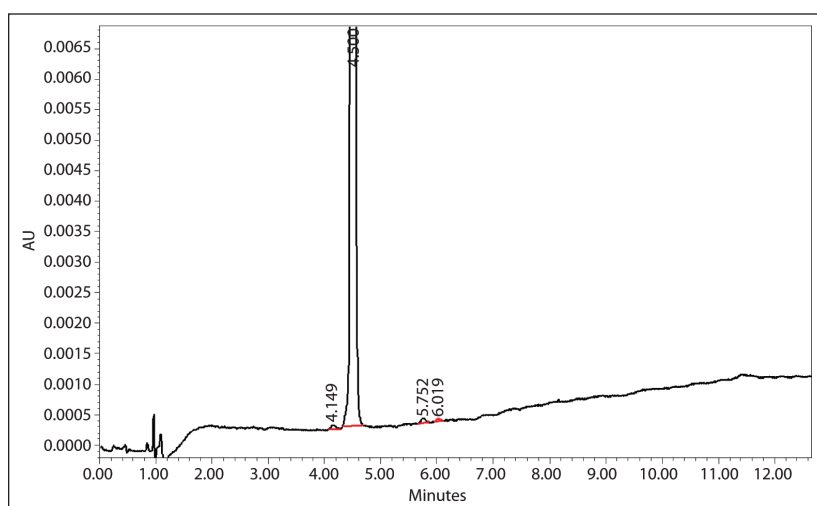


Figure 8. Analytical gradient separation of combined purified fraction.

To speed dry-down time, the system was used to concentrate the collected 92-mL fraction. The 92 mL collected was first diluted to 1 L with water. The column was then equilibrated with 99:1 water/acetonitrile. The entire diluted fraction was placed onto the column via the load valve embedded on the front of the pump. Once the entire sample was on the column, a simple step gradient to 100% acetonitrile was run and the eluted peak was captured in <10 mL, a 10X concentration factor. This small, mostly organic fraction was then dried to liberate crystalline puerarin.

CONCLUSIONS

Puerarin, an extract of kudzu root, was isolated and purified using Waters modular preparative HPLC system. Separations were analytically developed and geometrically scaled to two sizes of prep columns. The bulk purifications performed in an automated manner, eliminating the need for constant user intervention. Finally, the collected fractions were concentrated using the same system and column that was used to isolate the compound of interest.

- The system was shown to be flexible, running multiple columns (10 and 19 mm I.D.), using a variety of injection techniques (Autosampler, Line D, load valve), and easily adjustable fraction collection parameters using Empower 2 Software.
- Total system software control via Empower 2 Software provided system flexibility by allowing easy modification of all method parameters.
- The system was used for both purification and concentration steps without requiring modification to the system.
- The initial extract contained 50.0% puerarin and was purified to greater than 97.5%, and concentrated in a small volume ready for dry-down.

References

1. PDR for Herbal Medicines, 4th Ed., 2007; Herbal Monographs: 501-505.
2. Sarker SD, and Latif Z. Natural Products Isolation 2nd edition, 2006.
3. Aubin A, and Cleary R. Analytical HPLC to Preparative HPLC: Scale Up Techniques using a Natural Product Extract, Waters Application Note, 2009.

Waters

THE SCIENCE OF WHAT'S POSSIBLE.™

Waters and Alliance are registered trademarks of Waters Corporation. Empower, SunFire, OBD, and The Science of What's Possible are trademarks of Waters Corporation. All other trademarks are the property of their respective owners.

©2010 Waters Corporation. Produced in the U.S.A.
November 2010 720003797EN LL-PDF

Waters Corporation
34 Maple Street
Milford, MA 01757 U.S.A.
T: 1 508 478 2000
F: 1 508 872 1990
www.waters.com

