

Mobility Assisted Data independent, Relative Label-Free Protein Quantification

GOAL

The quantitative analysis of complex protein mixtures requires tryptic digestion coupled with a protein identification strategy that can accurately identify proteins with high reproducibility. This has often been overlooked and many quantitative measurements have been based upon spurious identifications. The depth to which a complex sample can be interrogated is also crucial as this defines the lowest abundance limit of proteins that maybe quantified. The SYNAPT® G2 HDMS™ System has substantial improvements in performance (mass resolution and accuracy, dynamic range, sensitivity, and mobility resolution). These enable highly accurate protein identification and label-free, relative protein quantification, which we present here.

BACKGROUND

Isotope-labeled and label-free protein quantification in increasingly complex proteomics samples is conducted to overcome the bias and difficulty of sample fractionation. This places a demand on the performance of the analytical LC/MS system, requiring the highest obtainable coverage of the proteins present within the sample in order to identify quantifiable, proteotypic information, without increasing the protein false discovery rate (FDR) and false quantification rate (FQR). As such, technology improvements are indispensable. The use of the SYNAPT G2 HDMS System and the results for the analysis of differentially spiked protein standards in a complex cell lysate from *Escherichia coli* (*E. coli*) are described.

Obtain highly accurate and specific information for label-free protein quantification using an IMS-enabled method.

THE SOLUTION

Three replicates of each *E. coli* sample, differentially spiked with bovine serum albumin (BSA), alcohol dehydrogenase (ADH), Enolase and Glycogen phosphorylase B were analyzed. The nominal ratios were 1:8, 1:1, 1:2, and 2:1, respectively. The peptides were separated and analyzed using a nanoACQUITY UPLC® System coupled with a SYNAPT G2 HDMS. The data were acquired in LC/HDMS^E mode – an unbiased mobility assisted TOF acquisition method – an unbiased mobility assisted TOF acquisition method – switching between low and elevated energy on alternate



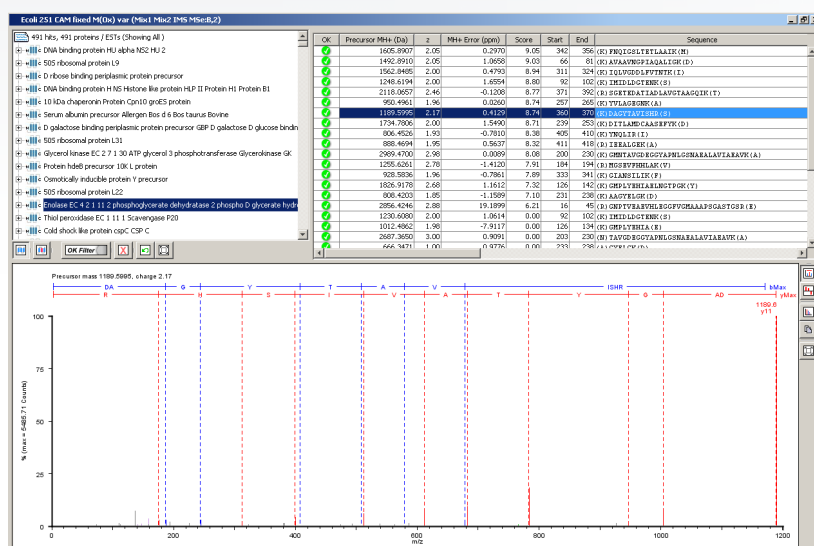


Figure 1. Qualitative LC-HDMS^E identification Enolase.

Figure 1 illustrates the qualitative results overview for an HDMS^E acquisition of one of the analyzed samples. In this particular instance, the on-column amount of highlighted Enolase was 12.5 fmol and the amount of *E. coli* digest equal to 200 ng. The results shown in Figure 2 demonstrate the relative quantification result for BSA. A graphical representation for all quantified proteins, including the protein spikes, is shown in Figure 3.

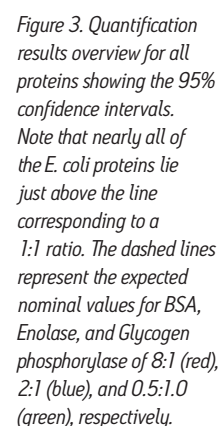

In this technical brief, we demonstrate an ion mobility-enabled data independent acquisition method for quantification of four protein standards, which were spiked into a biological background. The additional specificity of the IMS-enabled experiment provides highly accurate information for qualitative and quantitative experiments. All of the reported protein ratios are within a few percent of their nominal spike values and included in the reported 95% confidence intervals.

THE SCIENCE OF WHAT'S POSSIBLE.™

©2011 Waters Corporation Produced in the U.S.A.
March 2011 720003881en AG-PDF

Waters Corporation
34 Maple Street
Milford, MA 01757 U.S.A.
T: 1 508 478 2000
F: 1 508 872 1990
www.waters.com

