

The Analysis of Coccidiostatic Agents in Feed Using the ACQUITY UPLC I-Class and Xevo TQ-S

Nathalie Gillard,¹ Gilles Pierret,¹ Philippe Delahaut,¹ Marijn Van Hulle²

¹Centre d'Economie Rurale, Marloie, Belgium

²Waters Belgium

APPLICATION BENEFITS

A fast, robust, accurate, and sensitive method for 11 coccidiostats in feed samples was developed on an ACQUITY UPLC I-Class® System with Xevo® TQ-S.

- Compared to the original HPLC/MS-MS method the feed sample extracts can be further diluted by a factor of 50, using only half of the injection volume.
- Runtime reduced from 16 min. (HPLC/MS-MS) to eight min. (UPLC/MS-MS).
- RADAR™ provides the necessary qualitative information about possible matrix effects and is therefore a valuable tool during method development.

WATERS SOLUTIONS

ACQUITY UPLC I-Class

Xevo TQ-S

ACQUITY UPLC BEH Columns

MassLynx® Software

TargetLynx™ Application Manager

KEY WORDS

Coccidiosis, animal feed, coccidiostat, veterinary drug, coccidiostatic agents

INTRODUCTION

Coccidiosis is a parasitic disease of the intestinal tract of animals caused by coccidian protozoa. The disease spreads from one animal to another by contact with infected feces or ingestion of infected tissue. Diarrhea, which may become bloody in severe cases, is the primary symptom. Most animals infected with coccidia are asymptomatic; however, young or immuno-compromised animals may suffer severe symptoms, including death. Among domestic animals, industrially bred poultry and rabbits are particularly prone to this disease.

Today 11 coccidiostatic agents are authorized as feed additives in accordance with EU Regulation 2003/1831/EC. Other regulations specify which agents can be used for specific animal species. Because feed companies typically use the same production line for the production of different feeds, carryover and therefore transfer of coccidiostats from one batch to another is unavoidable. Despite the efforts taken by the feed companies to avoid any cross-contamination, as imposed by European directive 2005/183/EC, maximum levels of coccidiostat carryover have been set (2009/8/CE) to protect animal health and guarantee minimal risk to the consumers. This directive sets maximum carryover levels of 1% for sensitive animal species and 3% for less-sensitive non-target animal species, respectively. These required LOQ levels, described in Table 1, which are drug dependent, are based on an extraction protocol described further. These levels are very diverse, making it difficult to combine all of the components into one multi-residue analysis and achieve good overall sensitivity, accuracy, and linear range.

In addition feeds are very complex and diverse mixtures. In a routine environment, it is impossible to use matrix matched calibration or standard addition for each type of feed. Instead internal standards and one feed matrix are used. The method accuracy is then validated by selecting different feed matrices and performing spike recovery experiments at different levels with a quantitation of the results based on one feed matrix.

	Max. therapeutic dose	Max. value at 1% carry-over	Max. value at 3% carry-over	Required LOQ
Coccidiostat	[mg/kg]	[µg/kg]	[µg/kg]	[µg/kg]
Lasalocid	125	1250	3750	312.5
Narasin	70	700	2100	175.0
Salinomycin	70	700	2100	175.0
Monensin	125	1250	3750	312.5
Maduramicin	5	50	150	12.5
Semduramicin	25	250	750	62.5
DNC, Nicarbazin	50	500	1500	125.0
Diclazuril	1	10	30	2.5
Decoquinate	40	400	1200	100.0
Halofuginone	3	30	90	7.5
Robenidine	66	700	2100	175.0

Table 1. Therapeutic dose, carry-over levels, and required LOQ for the 11 coccidiostats.

It is known that matrix components can significantly alter the response in electrospray ionization, either a signal enhancement, but most likely signal suppression. Matrix effects are minimized by reducing the absolute amount of matrix ions in the source region. One way that this can be achieved is to dilute the samples (if this method used is sensitive enough to permit this) and hence reduce the matrix loading on-column. As a consequence of this approach, when working in a routine food and feed testing laboratory, it can also be observed that the instrument will require less frequent cleaning and therefore better instrument uptime and method robustness.

This application note describes a fast, accurate, and robust UPLC/MS-MS method using Waters® ACQUITY UPLC I-Class System with Xevo TQ-S for the detection of 11 coccidiostatic agents in feed at levels down to 0.25% carryover levels. The Xevo TQ-S is a highly sensitive tandem quadrupole instrument with fast positive/negative ion switching capabilities able to deal with challenging matrices.

EXPERIMENTAL

Sample preparation

This method was previously employed on a HPLC-MS-MS and has been transferred to appropriate conditions for UPLC®, and also includes the addition of a final dilution step.

1. Weigh 5 g of ground and homogenized feed sample into a 50-mL disposable centrifuge tube.
2. Spike with 50-µL internal standard pool (50 µg/mL robenidine-d8 and nigericine, 25 µg/mL DNC-d8, 5 µg/mL diclazuril-bis and decoquinate d5).
3. Add 10 mL of a 10% Na₂CO₃ solution and hand shake.
4. Add 15 mL acetonitrile
5. Shake for 30 minutes.
6. Centrifuge 5 minutes at 2000 rpm (4 °C).
7. Transfer the supernatant into a 50-mL tube.
8. Repeat the acetonitrile extraction and combine both organic extracts.
9. Transfer 1 mL of extract in a glass tube and dilute the samples 50 times in initial mobile phase.

UPLC conditions

System:	ACQUITY UPLC I-Class
Column:	ACQUITY BEH C ₁₈ 2.1 x 100 mm
Column Temp.:	50 °C
Sample Temp.:	10 °C
Injection:	10 µL
Mobile phases:	A Water 0.1% formic acid B Methanol 0.1% formic acid

The gradient is shown in Table 2.

MS conditions

MS system:	Xevo TQ-S	<u>Time</u>	<u>% A</u>	<u>% B</u>	<u>?</u>
Polarity:	ES +/-	0.0	50	50	—
Capillary voltage (kV):	1.00 in positive ion ES and 3.00 in negative ion ES	0.5	50	50	6
		3.0	0	100	6
		5.0	0	100	6
Source temp.:	150 °C	7.0	50	50	1
Desolvation temp.:	500 °C	8.0	50	50	1
Cone gas flow:	150 L/hr				
Desolvation gas flow:	1200 L/h				

Compound tuning was accomplished using IntelliStart™ Software. IntelliStart automatically generates up to 5 MRM transitions per compound on the basis of either a compound mass or its elemental composition. The advantage is fact that multiple adducts can be selected simultaneously. This is particularly interesting for coccidiostatic agents that easily form sodium adducts. A screenshot of the IntelliStart wizard is shown in Figure 1. An extract of optimized MRM transitions for maduramycin can be found in Figure 2.

IntelliStart Setup Parameters

Sample Tune and Develop Method

Compound Details

Compound Name	Molecular Mass/Formula	Adduct A+	Adduct B+	Adduct A-	Adduct B-
<input type="checkbox"/> Maduramycin	C ₄₇ H ₈₀ O ₁₇	[M+H] ⁺	[M+Na] ⁺	[M-H] ⁻	
<input type="checkbox"/>					
<input type="checkbox"/>					
<input type="checkbox"/>					

☐ Multiply Charged Parents

Method Details

☐ Create New Sample Tune ☒ Load Existing Sample Tune

Sample Tune Name: C:\MASSLYNX PROJECTS\Coccidiostatics.PRO\

☐ Develop SIR method: C:\MASSLYNX PROJECTS\Coccidiostatics.PRO\

☒ Develop MRM method: C:\MASSLYNX PROJECTS\Coccidiostatics.PRO\

☐ Keep HTML Name: Maduramycin

☐ Invoke Manual Optimisation

☐ Export To LC/MS System Check

☒ Append to existing methods

☐ Print to Printer ☐ Print to PDF

Optimization Ranges

Cone Voltage: Default (2 - 100) V

Collision Energy: Default (2 - 80) eV

Daughter ion settings

Number of MRM transitions per compound: 5

Lowest Fragment Ion Mass: 50.0 Da

Fluidics

Flow Path: Combined

Sample Reservoir: A

Sample Flow Rate: 10.0 µl/min

Figure 1. Screenshot of the IntelliStart wizard for maduramycin with elemental composition C₄₇H₈₀O₁₇.

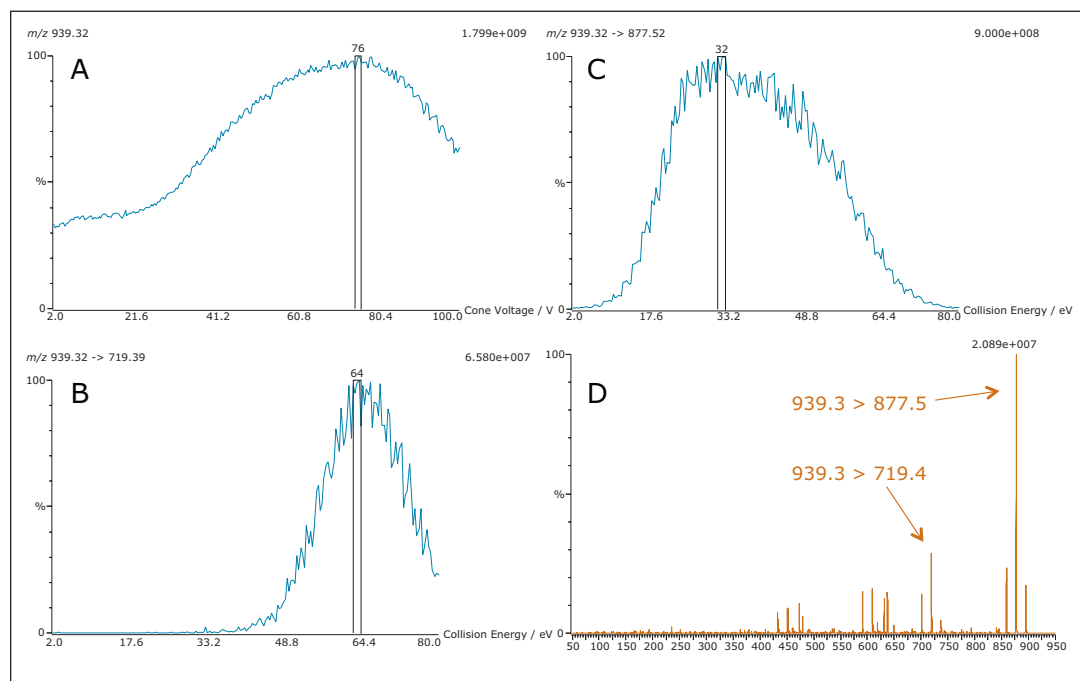


Figure 2. Extract from IntelliStart method development report showing optimization of cone voltage (A), optimization of collision energy for two transitions (B, C), and location of product ions (D) for the sodium adduct of maduramycin.

A separate MS function was automatically created for every individual compound. Table 3 shows an overview of all MRM transitions, including optimal cone voltage and collision energy. Two or three MRM transitions were chosen per component, except for the internal standards.

	Precursor mass <i>m/z</i>	Product mass <i>m/z</i>	Dwell time (s)	Cone voltage (V)	Collision energy (eV)
Robenidin	334.2	155.2	0.017	20	20
	334.2	111.1	0.017	20	40
Halofuginone	416.1	100.2	0.017	20	20
	416.1	120.2	0.017	20	20
Decoquinat	418.3	204.1	0.015	20	35
	418.3	372.3	0.015	20	20
Lasalocid	613.4	377.4	0.015	20	35
	613.4	577.4	0.015	20	30
Monensin	693.5	461.4	0.015	20	50
	693.5	501.4	0.015	20	50
Salinomycin	773.6	431.4	0.015	20	50
	773.6	531.4	0.015	20	40
Narasin	787.6	431.3	0.015	20	50
	787.6	531.3	0.015	20	45
Semduramycin	895.5	833.6	0.015	20	30
	895.5	851.6	0.015	20	35
Maduramycin	939.5	877.6	0.015	20	32
	939.5	719.5	0.015	20	64
DNC	301.2	137.1	0.017	20	15
	301.2	107.1	0.017	20	35
Diclazuril	407.1	336.1	0.017	50	17
	405.1	334.1	0.017	50	17
Diclazuril-bis	421.1	323.1	0.017	50	25
DNC-D8	309.2	141.1	0.017	20	15
Robenidine-d8	342.2	142.3	0.017	20	25
Nigericine	747.5	703.5	0.015	20	55
Decoquinat-D5	423.3	377.3	0.015	20	20

Table 3. MS method parameters for the 11 coccidiostats and their internal standards.

Figure 3A shows the MassLynx MS method editor with retention time windows for each of the components. Figure 3B shows a typical function containing decoquinatone and its internal standard.

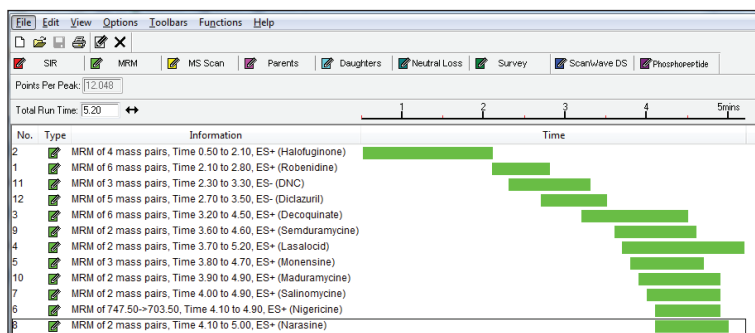


Figure 3A: MassLynx MS method editor with retention time windows.

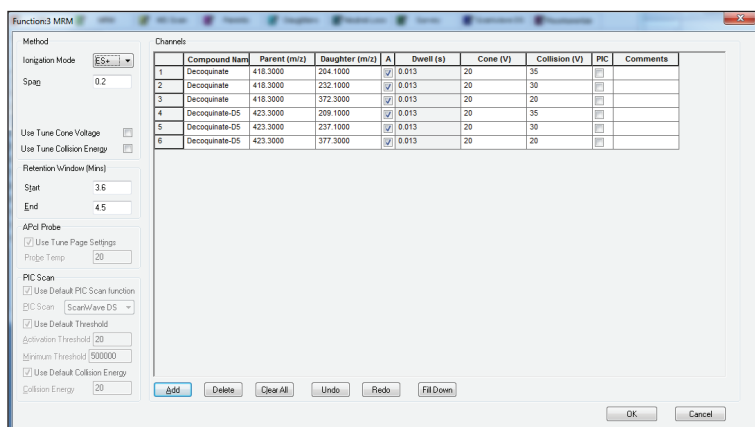


Figure 3B: MassLynx MS method function for decoquinatone and its internal standard.

RESULTS AND DISCUSSION

Original HPLC/MS-MS method

An HPLC/MS-MS chromatogram of a 1% carryover sample using the original HPLC method is shown in Figure 4A. The total runtime was 16 minutes.¹ There was an incomplete separation of the ionophore coccidiostats.

This method was then transferred to an ACQUITY I-Class System and the runtime was reduced without any significant effect on the spike recoveries. A typical chromatogram of a matrix-matched calibration standard at 1% carry-over level using this method is shown in Figure 4B. All 11 components eluted within a three-minute time frame. The overall method was eight minutes from injection to injection. Baseline separation was achieved for all components except for the pair lasalocid-maduramycin. There was clearly better separation of the ionophore coccidiostats.

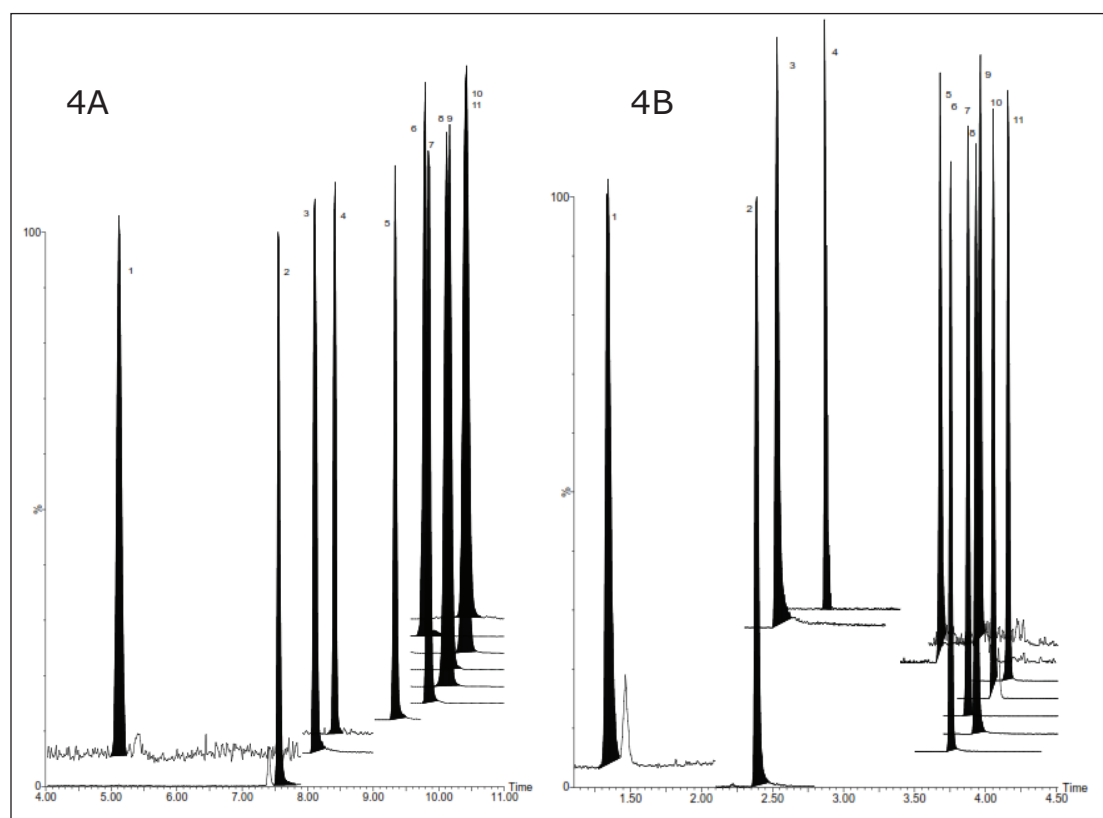


Figure 4A. HPLC/MS-MS chromatogram of a matrix-matched calibration standard at 1% carry-over level, showing Halofuginone (1), robenidin (2), DNC (3), diclazuril (4), decoquinat (5), semduramycin (6), lasalocid (7), salinomycin (8), monensin (9), narasin (10) and maduramycin (11). 4B. UPLC/MS-MS chromatogram of a matrix-matched calibration standard at 1% carry-over level, showing halofuginone (1), robenidin (2), DNC (3), diclazuril (4), decoquinat (5), semduramycin (6), lasalocid (7), salinomycin (8), monensin (9), narasin (10) and maduramycin (11).

Chromatographic method development – RADAR

The original HPLC method was transferred from an Alliance® HPLC System to an ACQUITY UPLC System. When using a UPLC method with a 3-minute gradient only, Semduramycin showed positive recoveries up to 200% in some of the feed QC samples relative to the matrix matched calibration standard. Using a 6-minute gradient, recoveries were within the acceptance criteria. By using the RADAR™ functionality on the Xevo TQ-S, MRM and full scan chromatograms were acquired simultaneously. As shown in Figure 5A, a matrix component is interfering at the same retention time as semduramycin, possibly giving rise to the observed matrix effect. In Figure 5B it is clear that the longer gradient time results in a better separation between semduramycin and the matrix component.

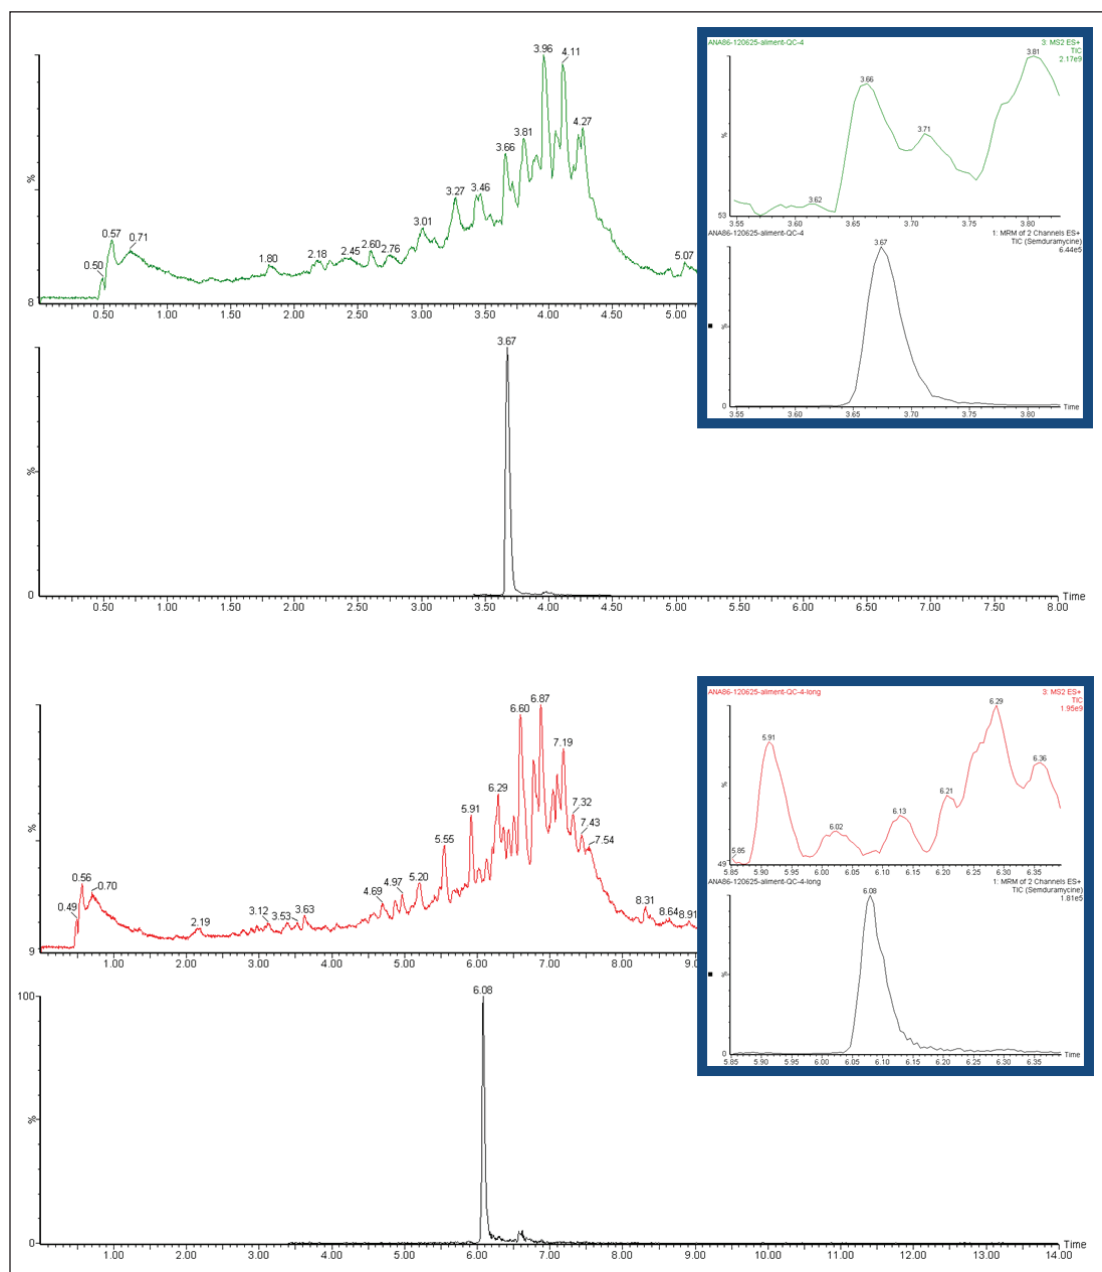


Figure 5A. MRM chromatogram of semduramycin (bottom trace) and Full scan TIC (top trace) with zoom on retention time zone of interest, showing a chromatographic interference at the retention time of semduramycin.

Figure 5B. MRM chromatogram of semduramycin (bottom trace) and full scan TIC (top trace) with zoom on retention time zone of interest, showing a chromatographic separation of the interference at the retention time of semduramycin.

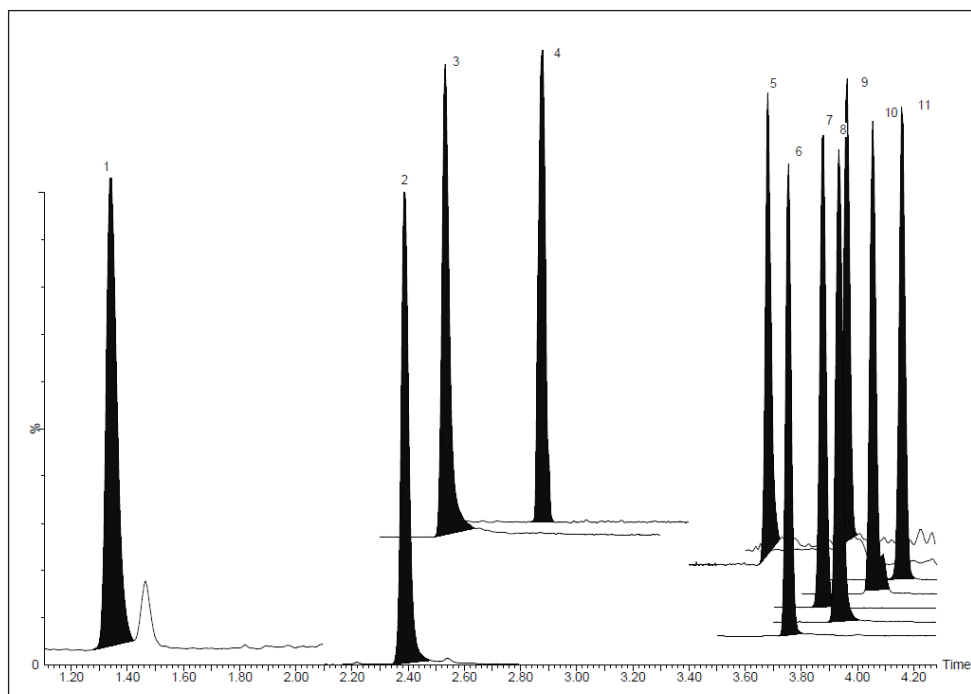


Figure 6. UPLC-MS-MS chromatogram of a matrix-matched calibration standard at 1% carryover level, showing Halofuginone (1), robenidin (2), DNC (3), diclazuril (4), semduramycin (5), decoquinate (6), monensin (7), lasalocid (8), maduramycin (9), salinomycin (10) and narsin (11).

Matrix effects – RADAR

We tested to find out to what extent the 50x diluted sample was susceptible to matrix effects. In the absence of matrix effects in the 50x diluted extract, it would be possible to use solvent-based calibration curves instead of matrix-matched calibration curves. In order to do this, both blank feed extract and solvent were spiked with the same concentration of coccidiostats, corresponding to the 0.25% carry-over level. An aliquot of both spike addition samples was also diluted sample 50 times. Matrix effects were then calculated for both dilution states as the ratio of the peak area of the different compounds in the extract divided by the peak area of the compound in the solvent standard. The results are described in Table 4.

Compound	Retention time (minutes)	Matrix effect Undiluted sample	Matrix effect 50x diluted sample
Halofuginone	1.1	79%	45%
Robenidine	2.1	73%	12%
DNC	2.5	11%	-2%
Diclazuril	2.9	22%	5%
Semduramycin	3.7	50%	-5%
Decoquinate	3.8	36%	-6%
Monensin	3.9	48%	5%
Maduramycin	4.0	75%	2%
Lasalocid	4.0	28%	-21%
Salinomycin	4.1	3%	7%
Narasin	4.2	-5%	6%

Table 4. Matrix effects in undiluted and 50x diluted feed extract spiked at the 0.25% contamination level.

For the undiluted sample, matrix effects was less likely for the late eluting compounds and varied from virtually nothing (Narasin, Salinomycin, and DNC) to extremely high (halofuginone and maduramycin). In the case of undiluted extracts, it is clear that matrix-matched calibration curves are a must.

For the 50 times diluted samples, matrix effects were clearly reduced and all below 7%, except for the early eluting halofuginone (45%) and robenidine (12%). Lasalocid showed a 20% signal enhancement in the presence of 50 times diluted feed extract. It is therefore best to still use a matrix matched calibration curve.

As would be expected, the total ion current (TIC) in the case of the undiluted sample is significantly higher than the TIC in the chromatograms of the 50 times diluted sample. It can be concluded that matrix effects are highly reduced when the feed extracts are diluted 50 times. With the sensitivity of the Xevo TQ-S, these diluted feed samples can still be analyzed with good sensitivity. Analyzing smaller amounts of diluted samples will lead to less frequent cleaning and therefore better instrument uptime and better method robustness.

Sensitivity

At the 0.25% carryover level, even the most challenging components (halofuginone, diclazuril, maduramycin, and Semduramycin) can still be detected with signal-to-noise values above 20. The signal-to-noise was determined using raw data and a peak-to-peak noise definition. Taken into account the extraction procedure, the 0.25% carry-over levels corresponds to amounts injected on column that are shown in Table 5.

A chromatogram of a matrix-matched calibration standard at 0.25% carryover level with corresponding signal-to noise levels can be found in Figure 6.

0.25% Carryover calibration standard		
Name	Concentration (µg/kg)	Amount on column (pg)
Halofuginone	7.5	1.875
Robenidin	175	43.75
DNC	312.5	78.125
Diclazuril	2.5	0.625
Maduramycin	12.5	3.125
Monensin	312.5	78.125
Salinomycin	175	43.75
Narasin	312.5	78.125
Lasalocid	312.5	78.125
Semduramycin	62.5	15.625
Decoquinate	100	25

Table 5. Absolute amounts injected on column in the 0.25% carry-over calibration standard.

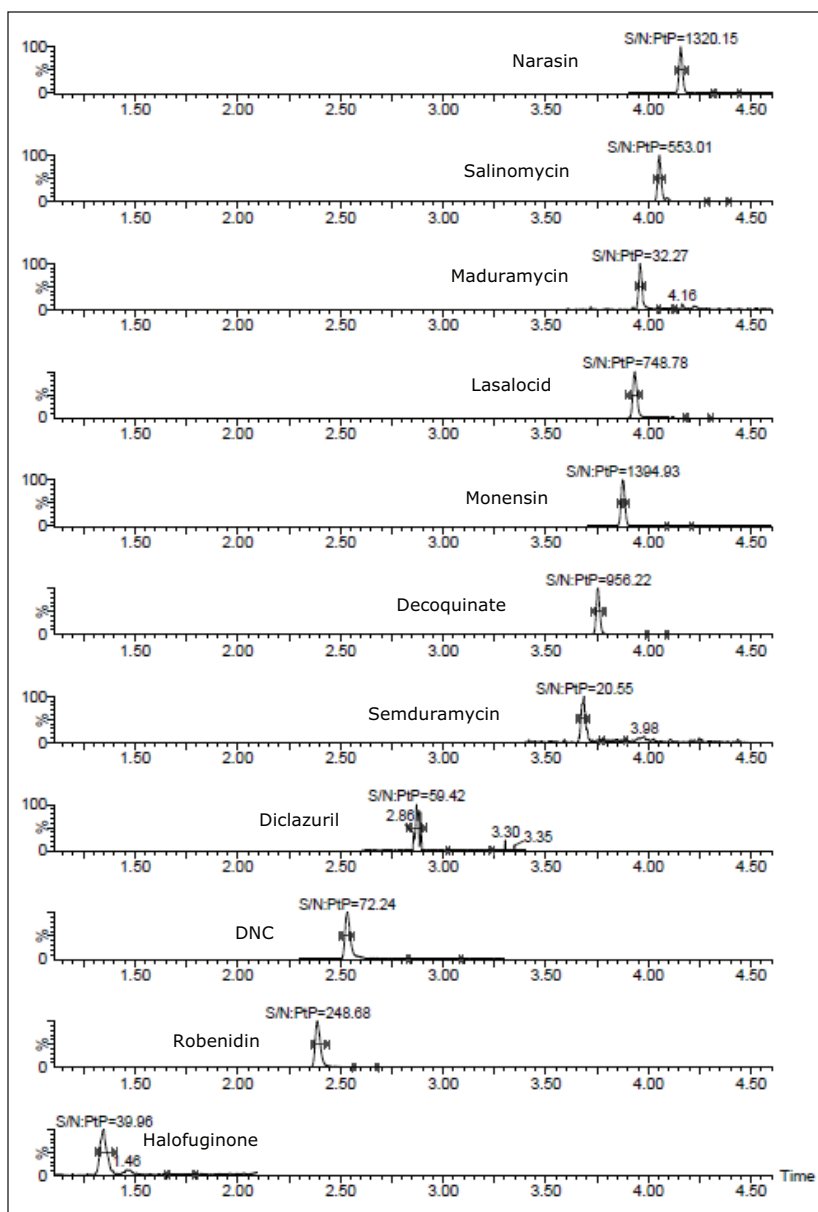


Figure 7. Chromatogram of a matrix-matched calibration standard at 0.25% carry-over level with signal-to-noise values.

Spike recovery and repeatability

Eight fortified samples at 0.5% (n=1), at 1% (n=4) and at 3% (n=3) carryover level were analyzed with an eight-point matrix-matched calibration curve ranging from 0.25% to 6% carryover level of the maximum authorized content. Spike recovery and repeatability were determined and fulfill requirements of EU Decision 2002/657/CE.

For repeatability six replicates were analyzed. The results are shown in Table 6. Repeatability at the 1% carryover level was excellent with %CV values below 10% except for diclazuril (15%).

Compound	CV (%)
Halofuginone	7.7
Robenidine	2.2
DNC	2.6
Diclazuril	15.0
Maduramycin	3.4
Monensin	4.2
Salinomycin	2.9
Lasalocid	5.6
Semduramycin	3.6
Decoquate	2.3

Table 6. %CV values for all 11 coccidiostats.

These values are in good agreement with those obtained via the original HPLC/MS-MS method.¹

For accuracy, spike recovery experiments were carried out. Recovery values are all within the acceptance criteria specified by EU Decision 2002/657/CE.

Linearity

Linearity was examined by injecting a eight-point calibration curve for all 11 compounds. Linearity was excellent and within the studied range with coefficients of determination values above 0.995. Of all 88 calibration points, deviations were within a $\pm 10\%$ range, except for 3 points with a maximum deviation of +14%. Examples of residual curves and calibration curves are shown in Figure 8 for robenidine, halofuginone, and diclazuril. Due to the higher ion counts of the Xevo TQ-S at the LOQ level, the accuracy and precision at these low detection levels was better compared to other instruments.

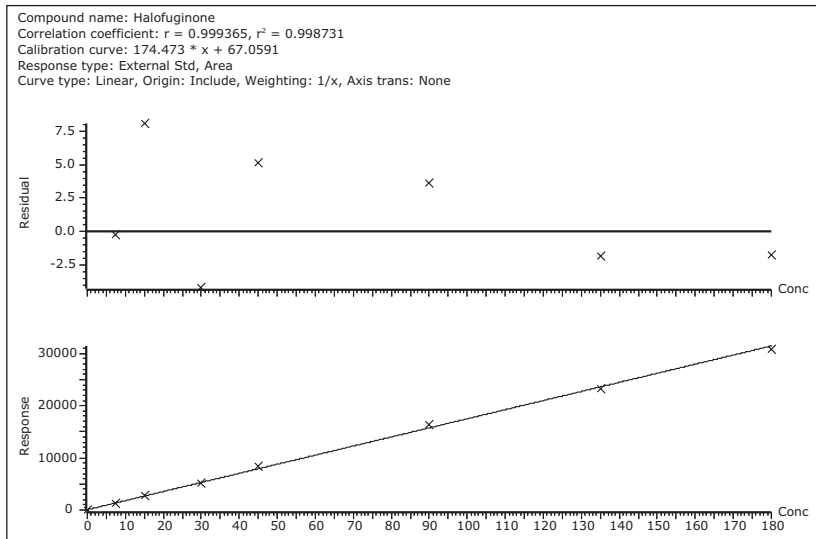


Figure 8A. Residuals curve and calibration curve for halofuginone.

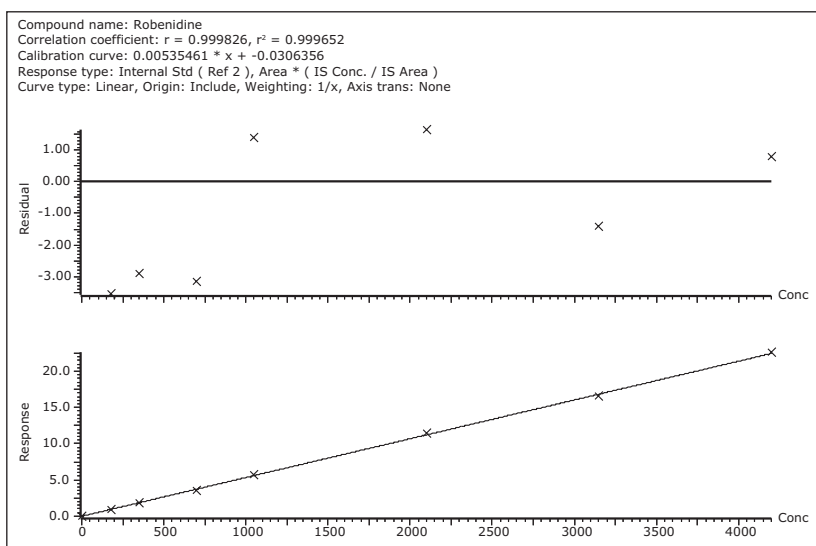


Figure 8B. Residuals curve and calibration curve for robenidin.

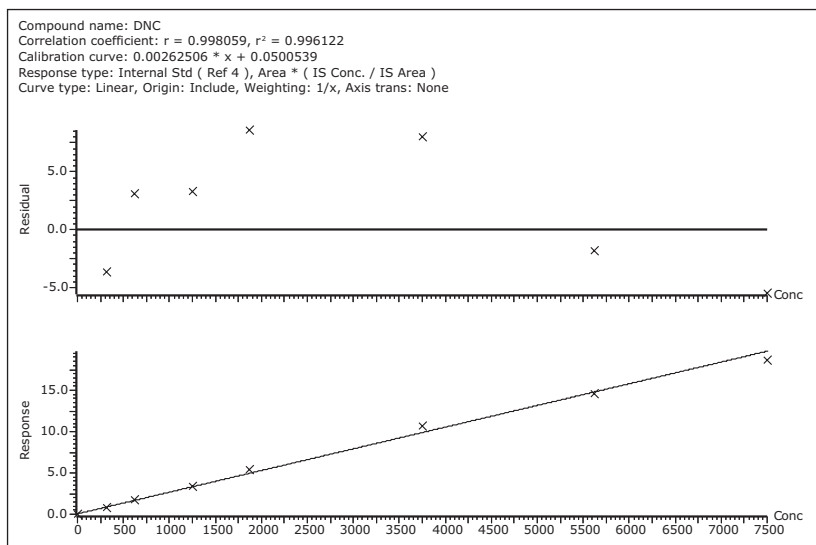


Figure 8C. Residuals curve and calibration curve for DNC.

CONCLUSIONS

A fast, robust, accurate, and sensitive method for 11 coccidiostats in feed samples was developed on an ACQUITY UPLC I-Class with Xevo TQ-S. Compared to the original HPLC/MS-MS method the feed sample extracts could be further diluted by a factor of 50, using only half the injection volume. This leads to less frequent instrument cleaning and therefore better instrument uptime and better assay robustness. RADAR provides the necessary qualitative information about possible matrix effects and is therefore a valuable tool during method development.

Reference

1. PH Delahaut, G Pierret, N Ralet, M Dubois and N Gillard. Multi-residue method for detecting coccidiostats at carry-over level in feed by HPLC-MS/MS. *Food Additives and Contaminants*. 27: 6, 801-809, June 2010.

Waters

THE SCIENCE OF WHAT'S POSSIBLE.®

Waters, ACQUITY UPLC, UPLC, Xevo, MassLynx, Alliance, and The Science of What's Possible are registered trademarks of Waters Corporation. TargetLynx and IntelliStart are trademarks of Waters Corporation. All other trademarks are the property of their respective owners.

©2013 Waters Corporation. Produced in the U.S.A.
August 2013 720004769en AG-PDF

Waters Corporation
34 Maple Street
Milford, MA 01757 U.S.A.
T: 1 508 478 2000
F: 1 508 872 1990
www.waters.com

