

CLICK ON THE UNDERLINED BLUE TEXT FOR DETAILS ON THE PRODUCTS USED IN THIS APPLICATION

TEST CONDITIONS

Chromatographic Conditions

Column: ACQUITY UPLC® BEH Amide
2.1 x 100 mm, 1.7 µm

Part Number: [186004801](#)

Mobile Phase A: 80/20 MeCN/H₂O with 0.2% triethylamine [TEA]

Mobile Phase B: 30/70 MeCN/H₂O with 0.2% triethylamine [TEA]

Flow Rate: 0.13 mL/min

Flow Profile: 90% A/10% B (75% MeCN with 0.2 % TEA)

Injection Volume: 1.3 µL (PLNO)

Sample Concentration: 1 mg/mL each

Sample Diluent: 50/50 MeCN/H₂O

Column Temperature: 35 °C

Strong Needle Wash: 20/80 MeCN/H₂O (800 µL)

Weak Needle Wash: 75/25 MeCN/H₂O (500 µL)

Seal Wash: 50/50 MeCN/H₂O

Instrument: Waters ACQUITY UPLC with ELSD

ELSD Conditions

Gain: 200

Pressure: 40 psi


Drift Tube Temperature: 40 °C

Nebulizer: Cooling


Data Rate: 10 pps

Filter Time Constant: Normal


STRUCTURES

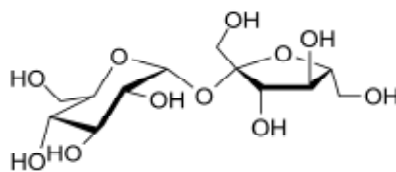



Sucrose




Fructose

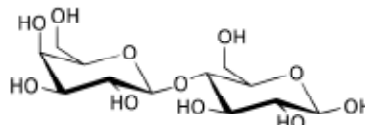

Lactose

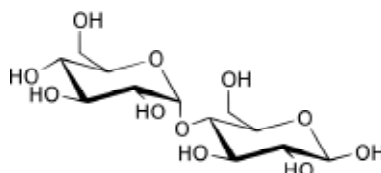p-Toluamide
(unretained compound)

Maltose



Glucose

COMPOUNDS

1. p-Toluamide
2. Fructose
3. Glucose
4. Sucrose
5. Maltose
6. Lactose

