CLICK ON THE UNDERLINED BLUE TEXT FOR DETAILS ON THE PRODUCTS USED IN THIS APPLICATION

TEST CONDITIONS

Chromatographic Conditions

Column:	ACQUITY UPLC® BEH Amide 2.1 x 100 mm, 1.7 µm
Part Number:	186004801
Mobile Phase A:	80/20 MeCN/H_2O with 0.20% triethylamine [TEA]
Mobile Phase B:	30/70 MeCN/H_2O with 0.20% triethylamine [TEA]
Flow Rate:	0.20 mL/min
Flow Profile:	95% A/5% B (77.5% MeCN with 0.20% TEA)
Injection Volume:	1.3 µL (PLNO)
Sample Concentration:	5 mg/mL
Sample Diluent:	50/50 MeCN/H_2O
Column Temperature:	35 °C
Strong Needle Wash:	20/80 MeCN/H_2O (800 µL)
Weak Needle Wash:	75/25 MeCN/H_2O (500 µL)
Seal Wash:	50/50 MeCN/H_2O
Instrument:	Waters ACQUITY UPLC with ELSD

ELSD Conditions

Gain:	200
Pressure:	40 psi
Drift Tube Temperature:	40 °C
Nebulizer:	Cooling
Data Rate:	10 pps
Filter Time Constant:	Normal

STRUCTURES



Steviol

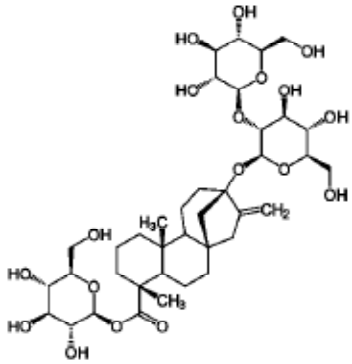

Stevioside

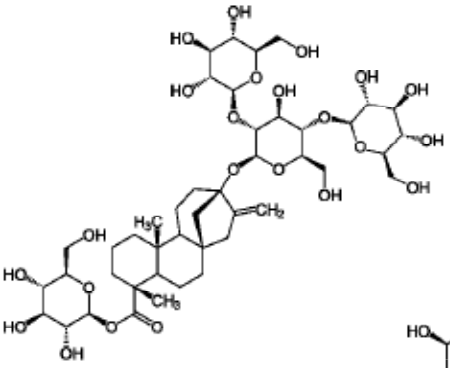

Rebaudioside A

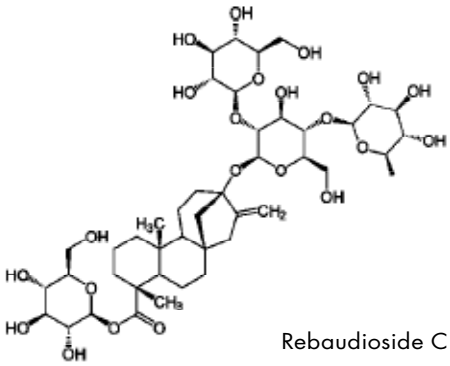

Rebaudioside C

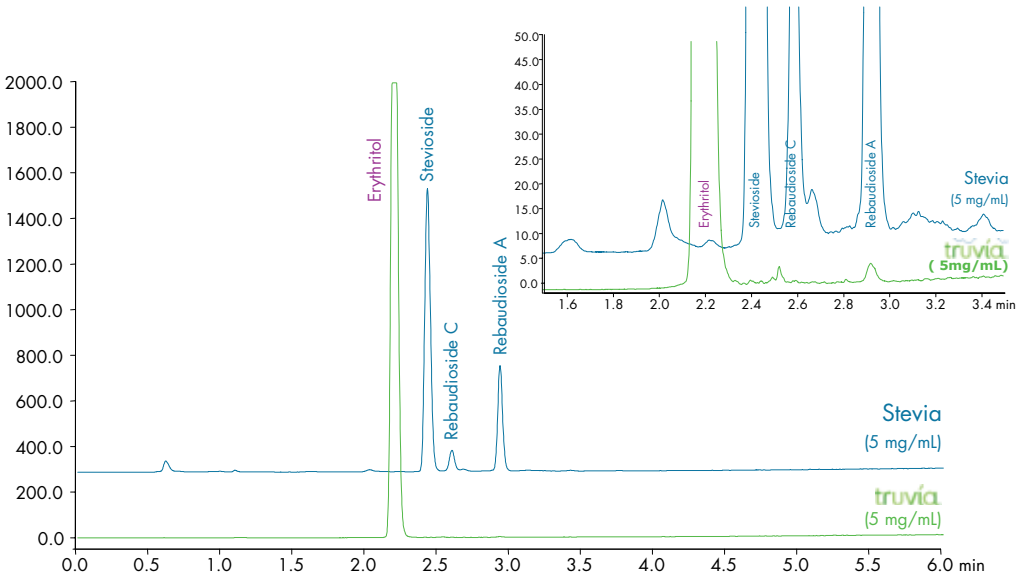

© 2009 Waters Corporation. Waters, ACQUITY UPLC and The Science of What's Possible are registered trademarks of Waters Corporation.