



# Clonazepam

## HPLC Method


**Column:** Symmetry® C<sub>18</sub>, 4.6 x 250 mm, 5 µm  
**Part number:** WAT054275  
**Mobile phase:** Water/methanol/acetonitrile 40:30:30  
**Flow rate:** 1.5 mL/min  
**Injection volume:** 25 µL of sample with 40 µg/mL of clonazepam and 80 µL/mL of o-dichlorobenzene (internal standard)  
**Detection:** UV @ 254 nm

### USP Tailing Factors

1. 1.08
2. 1.04

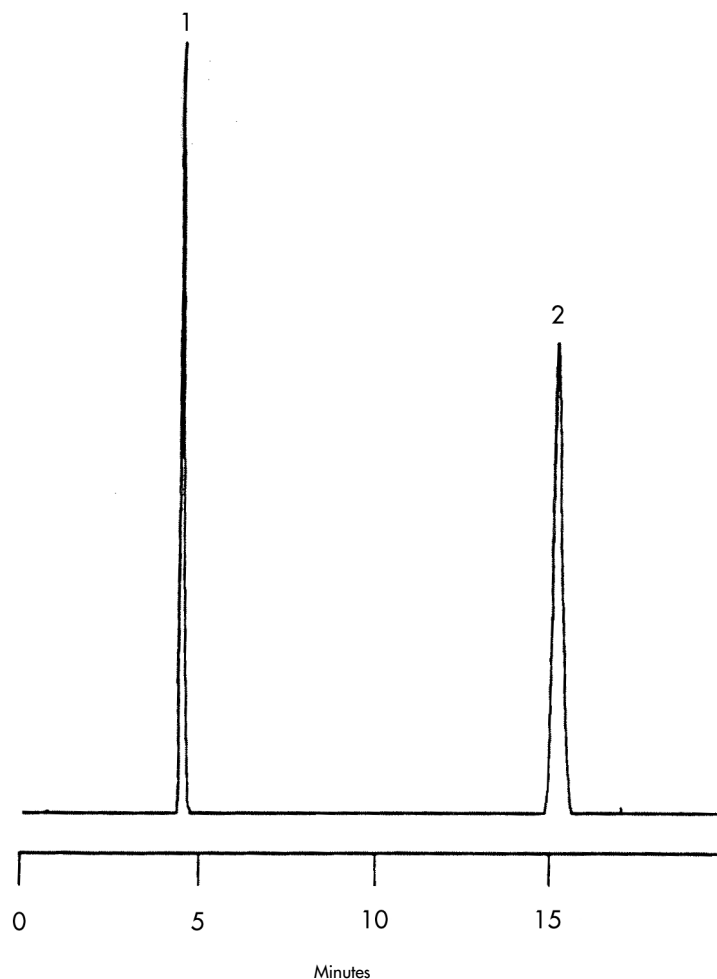

1. Clonazepam



2. O-dichlorobenzene (IS)