

# QUANTITATIVE ANALYSIS OF ACETYLCHOLINE ESTERASE ENZYME INHIBITION USING DIOS-TOF MS



Daniel B. Wall, Jeffrey W. Finch, and Steven A. Cohen  
Waters Corporation, 34 Maple St. Milford, MA USA

## INTRODUCTION

The pharmaceutical industry analyzes enzyme-inhibition reactions to determine the efficacy of a wide array of inhibitors. The ideal analytical technique for such work should be both quantitative and capable of a fast sample cycle time. A common example of enzyme-inhibition analysis is found in the case of Alzheimer's disease<sup>1,2</sup> where acetylcholine esterase inhibitors have been shown to lessen the effects of the disease. Inhibitors have been tested using traditional methods including microtiter plate-based fluorescence assays,<sup>3</sup> liquid chromatography (LC) mass spectrometry (MS)<sup>4,5</sup> and LC with UV absorption or fluorescence detection.<sup>4,6</sup> The fastest cycle times are achieved with the plate-based fluorescence assays though this method has limited analyte specificity. LC/MS-based approaches provide highly specific information but tend to have longer cycle times. Laser desorption based methods<sup>7,10</sup> have been used extensively for small molecule quantification including the MALDI based methods<sup>7,9,11-16</sup> and the matrix-free method of desorption/ionization on silicon (DIOS).<sup>8,10,17,18</sup> These approaches offer the potential for rapid cycle time combined with mass selectivity. The DIOS-TOF MS method is used in this work to quantify the rate of production of the choline product of the acetylcholine esterase reaction in the presence of the inhibitor tacrine. The results are compared between the DIOS-based method and the standard LC/MS/MS approach.

## GOALS

1. Determine the precision and accuracy of quantification of choline by DIOS-TOF MS and compare to LC/MS/MS
2. Measure the acetylcholine esterase  $K_m$  by DIOS-TOF MS
3. Find the  $IC_{50}$  for tacrine inhibition of the acetylcholine esterase reaction
4. Compare the DIOS-TOF MS and LC/MS/MS methods for analysis of enzyme-inhibition reactions

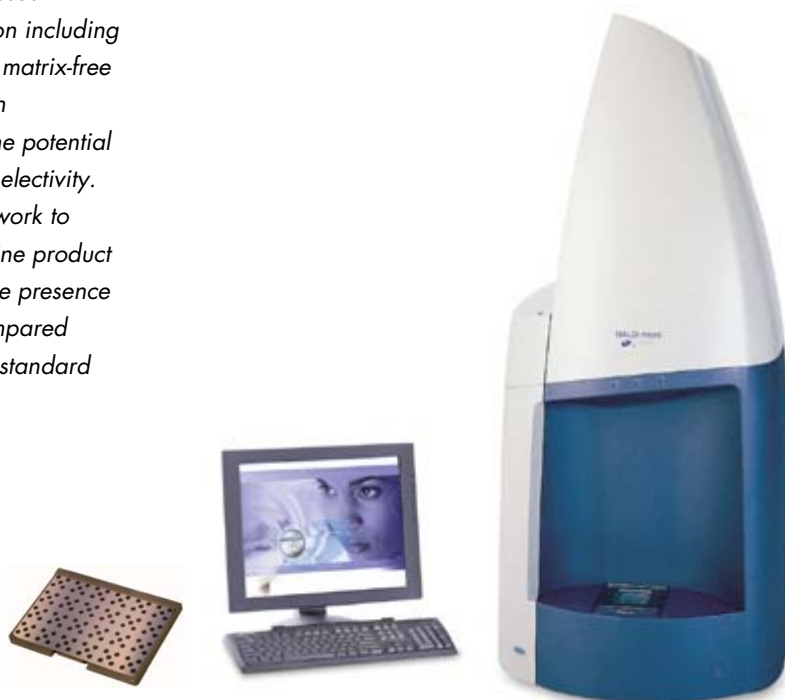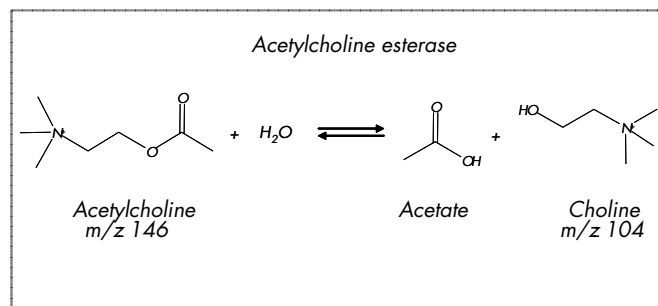

DIOS-TOF MS with the Waters Micromass® MassPREP™ DIOS-target™ Plate adds a new dimension to the capabilities of the Waters Micromass® MALDI micro MX™ Time-of-Flight Mass Spectrometer.

## EXPERIMENTAL

**Sample Preparation:** The enzyme reaction was typically run in 10mM ammonium bicarbonate and incubated at 37°C. The enzyme activity was quenched at specific time points by addition of one volume of acetonitrile containing the choline internal standard (choline\_d9: 90  $\mu$ M). This solution was either directly spotted onto the MassPREP DIOS-target Plate (0.4  $\mu$ L per well) or diluted 10-fold with water prior to LC/MS/MS (25  $\mu$ L per injection).

**DIOS-TOF MS:** 96 well MassPREP DIOS-target Plates were analyzed using a Micromass MALDI-TOF MS instrument operating in reflectron mode.

**LC/MS/MS:** LC/MS/MS analyses were performed on a Waters Micromass® Quattro micro™ equipped with an electrospray interface. The instrument was operated in MRM mode for detection of choline (104.1  $\rightarrow$  59.8) and the internal standard, choline\_d9 (113.2  $\rightarrow$  68.9).

### LC Conditions:

LC System	Alliance® HT 2795 XC Separations Module
Column	Waters Atlantis™ dC18 3 $\mu$ m 2.1 x 100 mm
Flow Rate	600 $\mu$ L/min. split to 150 $\mu$ L/min. into MS
Injection Volume	25 $\mu$ L
Gradient	Isocratic at 70% A and 30% B over 2 min. where A = 0.1% Formic Acid in Water, and B = 0.1% Formic Acid in Acetonitrile

### MS Conditions:

MS System	Micromass Quattro micro
Ion Mode	Positive
Cone Voltage	30 V
Desolvation Temp.	250°C
Source Temp.	120°C
Collision Energy	18 V
Detection Mode	MRM
Dwell	80 ms
Collision Gas	Argon, 2e <sup>3</sup> Torr

## RESULTS AND DISCUSSION

**Enzyme Kinetics:** Two critical parameters in the study of enzyme-inhibition reactions are the Michaelis constant ( $K_m$ ) and the fifty percent inhibition constant ( $IC_{50}$ ). The  $K_m$  is the substrate concentration at which the reaction occurs at half of the maximum rate and is an indicator of the affinity that an enzyme has for a given substrate. The  $IC_{50}$  is the concentration of inhibitor that reduces the enzyme reaction's initial velocity by half and is a measure of an inhibitor's efficacy.

**DIOS-TOF MS Quantification of Choline:** The standard calibration curve for choline is shown in Figure 1. The linear dynamic range extends from 5.0 to 500.0  $\mu$ M (3.8% RSD,  $R^2$  0.9976). Examples of the DIOS-TOF MS spectra are shown in Figure 2 for 100.0, 50.0, 20.0, 10.0 and 0.0  $\mu$ M concentrations of choline. Data were acquired by randomly sampling the target with the nitrogen laser and the final mass spectra were composed of 150 summed shots. The quantification was based on the MS peak intensity ratio of choline to choline\_d9.

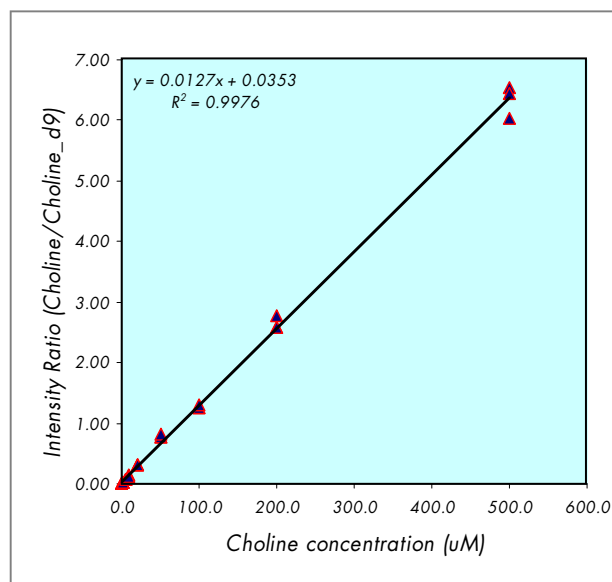


Figure 1. DIOS-TOF MS standard calibration curve for choline quantification (intensity ratio of choline to the internal standard choline\_d9 with the concentration of choline).

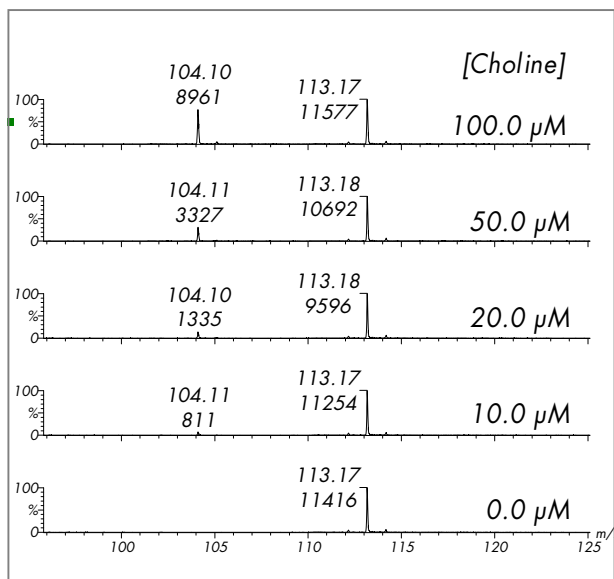


Figure 2. Examples of DIOS-TOF MS spectra showing choline ( $m/z$  104) from 100.0  $\mu\text{M}$  to 0.0  $\mu\text{M}$  with the internal standard choline\_d9 ( $m/z$  113) held at 90.0  $\mu\text{M}$ .

**LC/MS/MS Quantification of Choline:** The standard calibration curve for choline using LC/MS/MS extended from 1.0  $\mu\text{M}$  to 500.0  $\mu\text{M}$  (% RSD 1.6%,  $R^2$  0.999). The LC/MS/MS method performs better than the DIOS-TOF MS method in terms of linear dynamic range, % RSD and linear regression; however both methods are quantitative, and provide a means of assaying the acetylcholine esterase reaction.

**Michaelis Constant ( $K_m$ ):** Where  $V_0$  is the initial linear velocity of the reaction and  $[S]$  is the concentration of substrate, a plot of  $1/V_0$  vs.  $1/[S]$  generates a Lineweaver-Burk plot and a linear regression fit to this data is then used to estimate the  $K_m$  (Figure 3) at the x-intercept.

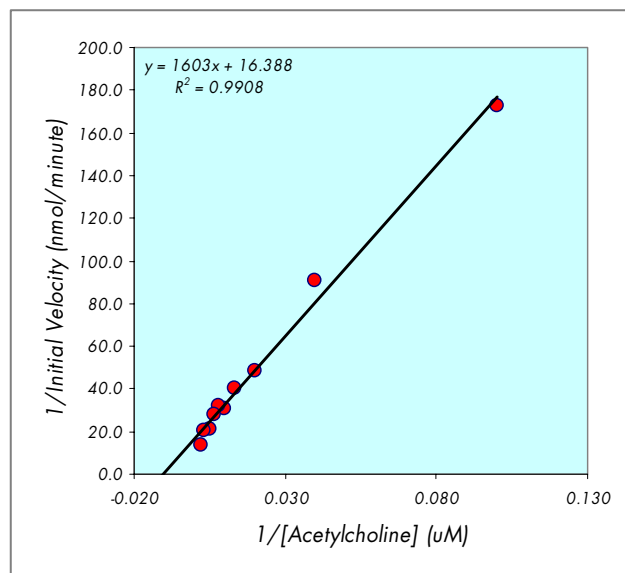


Figure 3. Lineweaver-Burk plot for acetylcholine esterase as determined from the DIOS-TOF MS data. This plot shows the reciprocal of the initial velocity ( $V_0$ ) vs. the reciprocal of the concentration of the substrate  $[S]$ , acetylcholine. The Michaelis constant ( $K_m = -1/x$  intercept) is calculated to be 97.8  $\mu\text{M}$  from this plot.

**Fifty Percent Inhibition Constant ( $IC_{50}$ ) for Tacrine:** With the acetylcholine concentration held at the Michaelis constant the reaction was run in the presence of the inhibitor tacrine at the following concentrations: 0.0, 0.1, 0.2, 0.5, 1.0, 2.0, 5.0, 10.0, 20.0, 50.0, 100.0, 200.0, 500.0, 1000.0, 2000.0, 5000.0, and 10000.0 nM. After quenching the reaction at thirty minutes the concentration of choline was determined. The plot of the concentration of choline vs. the log of the concentration of tacrine is shown in Figure 4 for DIOS-TOF MS and LC/MS/MS. The data clearly show a trend from no inhibition at low concentrations of tacrine to one hundred percent inhibition at high concentrations of tacrine. The midpoint between these two levels represents the fifty percent inhibition level and is used to calculate the  $IC_{50}$ .

With a third order polynomial fit to this data the concentration of inhibitor required for fifty percent inhibition of the enzyme, ( $IC_{50}$ ) can be estimated (Figure 4). The DIOS-TOF MS approach yielded a calculated  $IC_{50}$  of 32.0  $\pm$  0.2 nM while the LC/MS/MS method gave an  $IC_{50}$  of 31.8  $\pm$  0.1 nM. The reported  $IC_{50}$  value is 30.0 nM.<sup>1</sup> The DIOS-TOF MS and LC/MS/MS methods both result in  $IC_{50}$  values close to the reported value, demonstrating that DIOS is an effective technique for determining  $IC_{50}$  calculations.

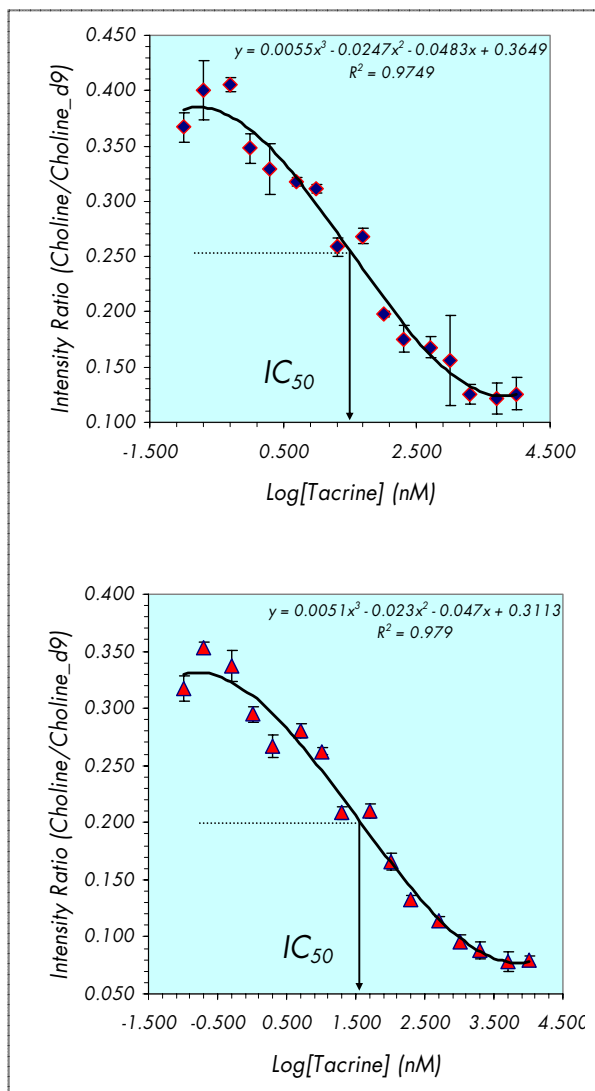


Figure 4. Calculation of the  $IC_{50}$  constant. The DIOS-TOF MS method (top) gives an  $IC_{50}$  of 32.0 nM while the LC/MS/MS method (bottom) gives an  $IC_{50}$  of 31.8 nM (reported  $IC_{50}$  = 30 nM)

## CONCLUSIONS

- The DIOS-TOF MS method is shown to be a rapid, simple approach to relative quantification for enzyme-inhibition  $IC_{50}$  assays.
- The linear dynamic range for choline, using DIOS-TOF MS, is from 5.0 to 500.0  $\mu$ M ( $R^2 = 0.998$ ) with an average relative standard deviation of 3.8%. Using LC/MS/MS, the linear dynamic range for choline is at least from 1.0 to 500.0  $\mu$ M choline ( $R^2 = 0.999$ ) with an average relative standard deviation of 1.6%.
- $IC_{50}$  values for tacrine were found to be 32.0 nM by DIOS-TOF MS and 31.8 nM by LC/MS/MS. Both are close to the reported value of 30.0 nM.
- Sample cycle time using DIOS-TOF MS was 40 seconds while that for LC/MS/MS was 2.1 minutes.
- The high throughput capabilities demonstrated by the DIOS-TOF MS technique may be applied to various screening applications where rapid, semi-quantitative results are desired.

**Further reading for complete experimental details:**

Wall, D, Finch J, Cohen C. Comparison of desorption/ionization on silicon (DIOS) time-of-flight and liquid chromatography tandem mass spectrometry for assaying enzyme-inhibition reactions. *Rapid Commun. Mass Spectrom.* 2004; in press.

**REFERENCES**

1. Costagli C, Galli A. *Biochem. Pharmacol.* 1998; 55: 1733-1737.
2. Kurz A. *J. Neural Transm. Suppl.* 1998; 54: 295-299.
3. Crespi C, Miller V, Penman B. *Anal. Biochem.* 1997; 248: 188.
4. Ayrton J, Plumb R, Leavens W, Mallet D, Dickens M, Dear G. *Rapid Commun. Mass Spectrom.* 1998; 12: 217.
5. Ayrton J, Dear G, Leavens W, Mallet D, Plumb R. *Rapid Commun. Mass Spectrom.* 1997; 11: 1953.
6. Masimirembwa C, Otter C, Berg M, Jonsson M, Leidvik B, Jonsson E, Johansson T, Backman A, Edlund A, Andersson T. *Drug Metab. Dispos.* 1999; 21: 1117.
7. Hatsis P, Brombacher S, Corr J, Kovarik P, Volmer D. *Rapid Commun. Mass Spectrom.* 2003; 17: 2303-2309.
8. Go E, Shen Z, Harris K, Siuzdak G. *Anal. Chem.* 2003; 75: 5475-5479.
9. Cohen L, Gusev A. *Anal. Bioanal. Chem.* 2002; 373: 571-586.
10. Huikko K, Ostman P, Sauber C, Mandel F, Grigoras K, Franssila S, Kotiaho T, Kostianen R. *Rapid Commun. Mass Spectrom.* 2003; 17: 1339-1343.
11. Kang M, Tholey A, Heinze E. *Rapid Commun. Mass Spectrom.* 2000; 14: 1972-1978.
12. Mims D, Hercules D. *Anal. Bioanal. Chem.* 2004; EPub.: 1618-2650.
13. Grant G, Frison S, Yeung J, Vasanthan T, Sporns P. *J. Agric. Food Chem.* 2003; 51: 6137-6144.
14. Frison-Norrie S, Sporns P. *J. Agric. Food Chem.* 2002; 50: 2782-2787.
15. Wang J, Sporns P. *J. Agric. Food Chem.* 1999; 47: 2009-2015.
16. Bucknall M, Fung K, Duncan M. *J. Am. Soc. Mass Spectrom.* 2002; 13: 1015-1027.
17. Lewis W, Shen Z, Finn M, Siuzdak G. *Int. J. Mass Spectrom.* 2003; 226: 107.
18. Thomas J, Shen Z, Crowl J, Finn M, Siuzdak G. *PNAS* 2001; 98: 4932-4937.
19. Al-Jafari A, Kamal M, Alhominida A. *J. Biochem. Mol. Toxicol.* 1998; 12: 245-251.
20. Alhominida A, Al-Rajhi A, Kamal M, Al-Jafari A. *Toxicology* 2000; 147: 33-39.

**WATERS CORPORATION**

34 Maple St.

Milford, MA 01757 U.S.A.

T: 508 478 2000

F: 508 872 1990

[www.waters.com](http://www.waters.com)

**Opt-In!** My Profile  
[www.waters.com](http://www.waters.com)

Waters, Micromass, DIOS-target, MassPREP, MALDI micro MX, Alliance, Quattro micro, and Atlantis are trademarks of Waters Corporation.  
All other trademarks are the property of their respective owners.  
©2004 Waters Corporation Produced in the U.S.A.

